

Sample Name :Glucagon (1-29), Human  
 Cat No: RP10772  
 Lot No : E2657020K  
 Time Processed :11:12:06 AM  
 Month-Day-Year Processed :12/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

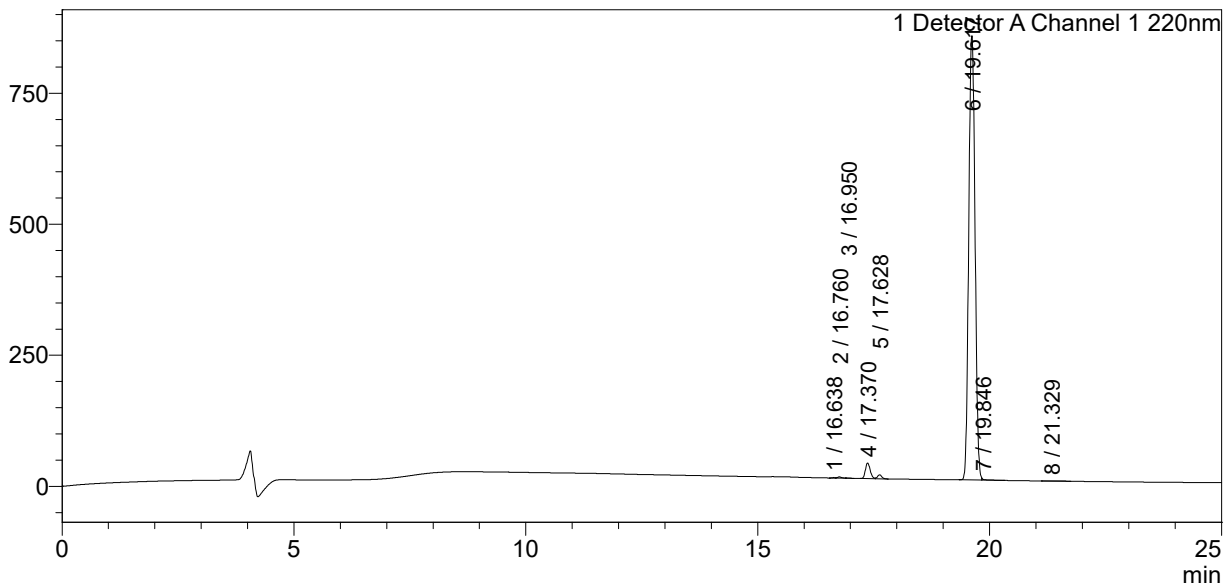

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.638	4089	775	0.049
2	16.760	13278	2188	0.161
3	16.950	1653	319	0.020
4	17.370	216355	29734	2.618
5	17.628	47950	7602	0.580
6	19.617	7962418	847843	96.356
7	19.846	11226	2645	0.136
8	21.329	6543	300	0.079
Total		8263512	891404	100.000