


Mass Spectrum

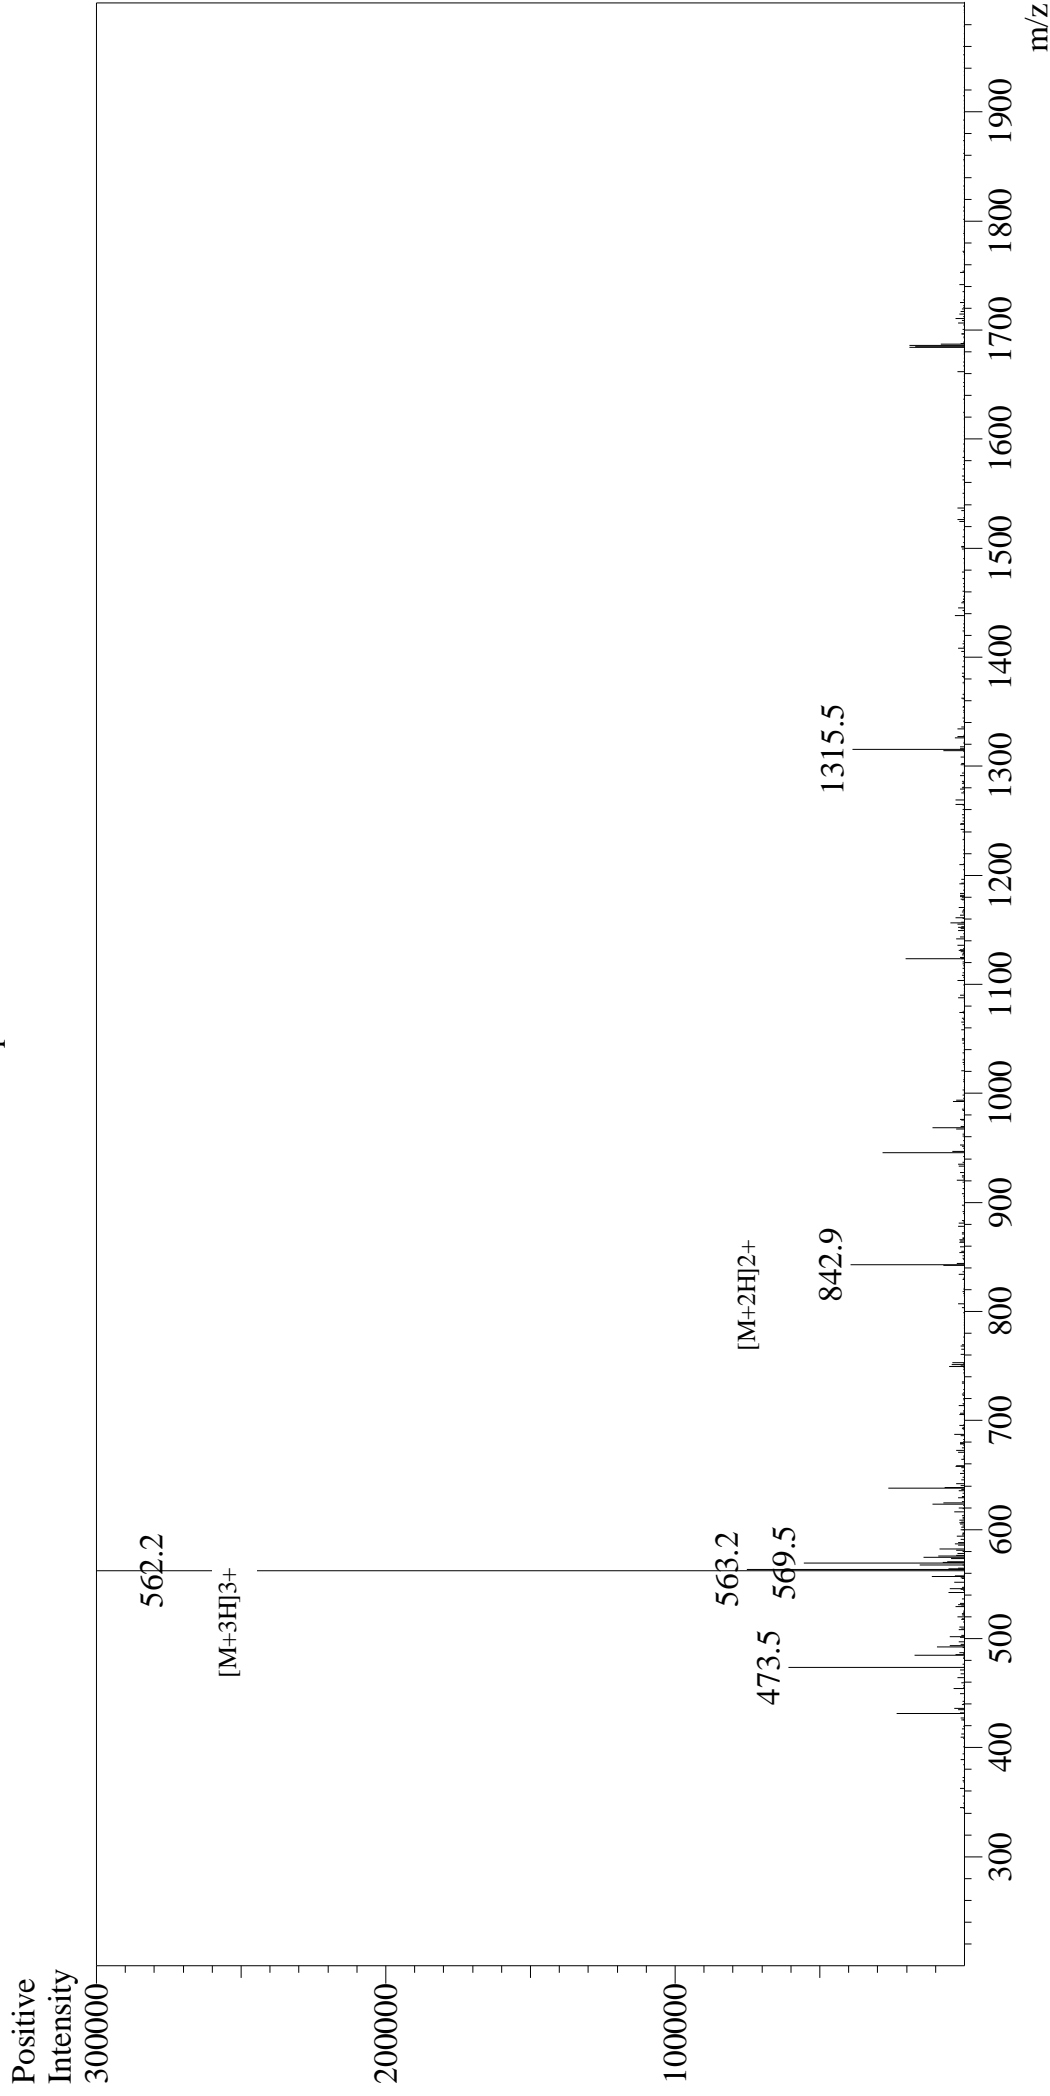

Sample Information

User : Gary
Month-Day Processed : 09/20/18
Time Processed : 17:10:42
Injection Volume : 0.2
Sample Name : α -Factor Mating Pheromone, yeast
Cat No. : RP01002
Lot No. : PE3841809
Theoretical MW : 1683.98
Observed MW : 1683.6

Interface

:ESI
Nebulizing Gas Flow :1.5L/min
CDL Temp :250°C
Block Temp :200°C

Equipment

: GK11010007
Interface Bias :+4.5kV
Drying Gas Flow :5 L/min
T.Flow :0.2ml/min
B.conc :50%H2O/50%MeOH