

Sample Name : hgp100(25-33)  
 Cat. No. : RP20344  
 Lot. No. : PE5391611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

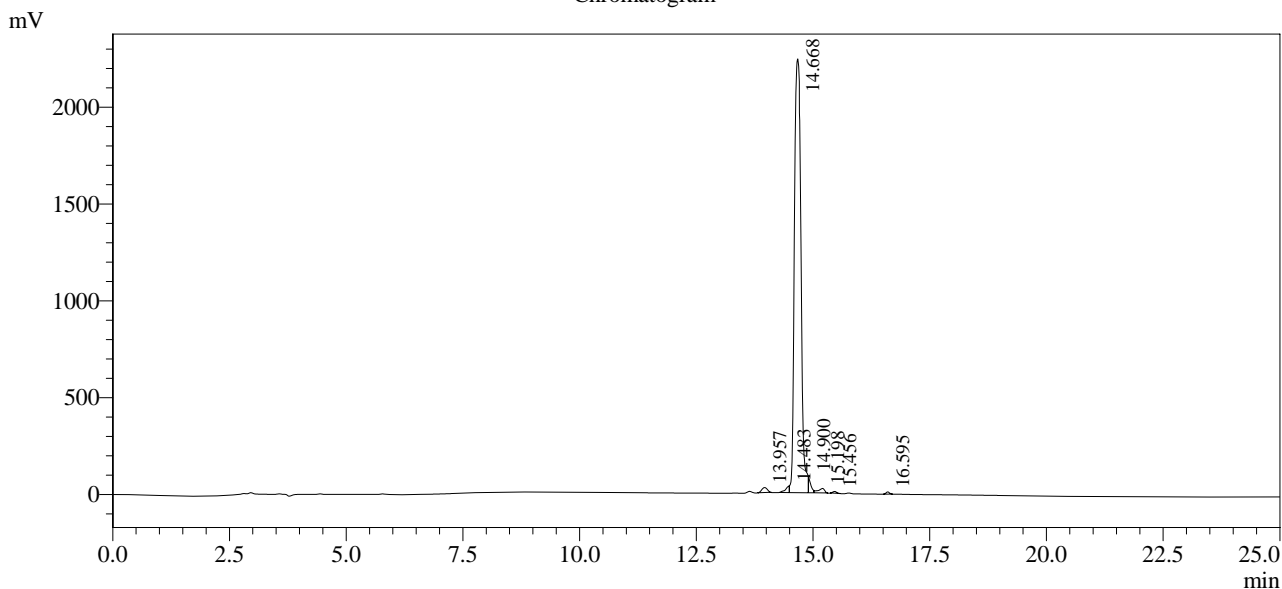

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.957	213176	25751	0.930
2	14.483	192915	33736	0.842
3	14.668	21910757	2240073	95.589
4	14.900	269476	85593	1.176
5	15.198	225486	22735	0.984
6	15.456	50824	8896	0.222
7	16.595	59157	11445	0.258
Total		22921792	2428228	100.000