


Mass Spectrum

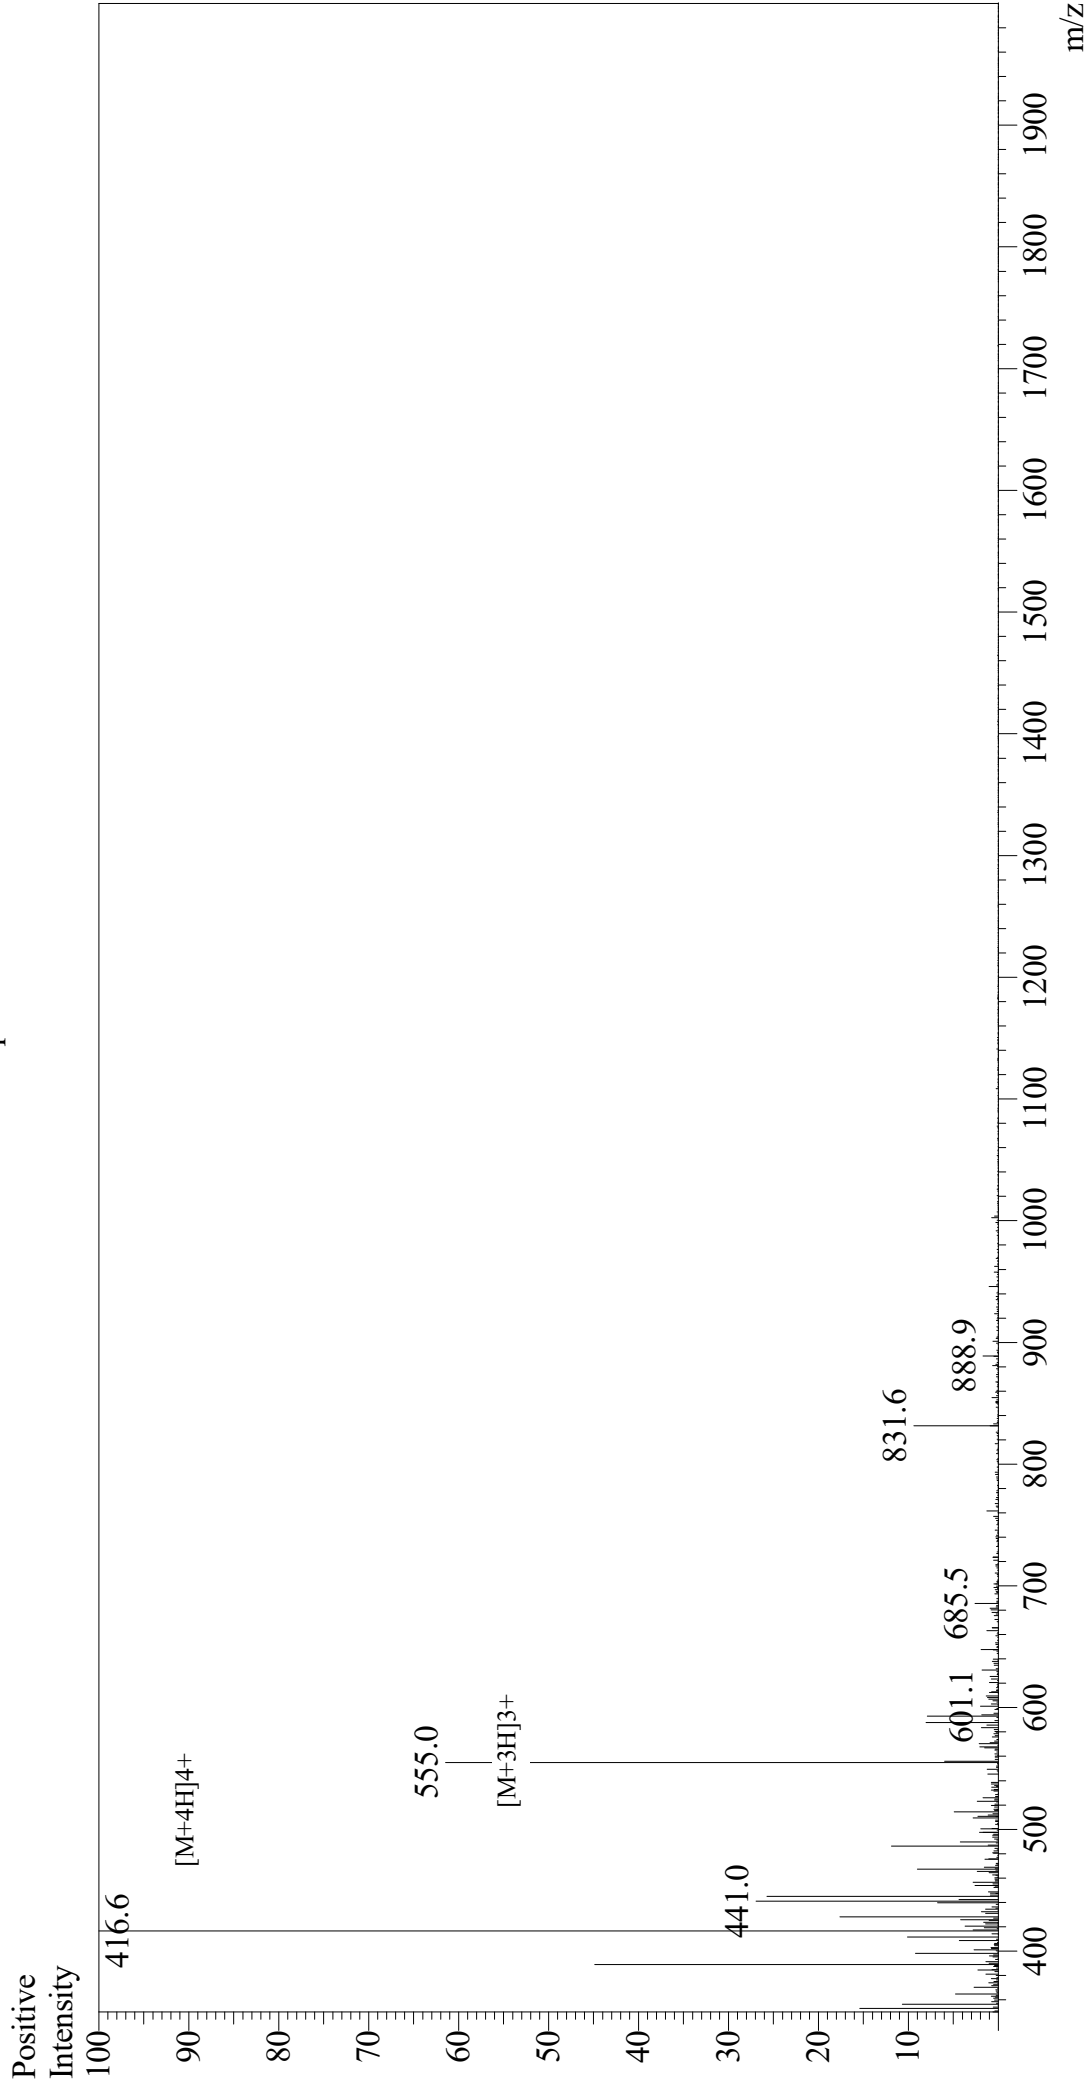

Sample Information
Month-Day Processed : 03/17/21
Time Processed : 17:10:11
Injection Volume : 0.4
Sample Name : Cys-TAT(47-57)
Cat. No. : RP20343
Lot. No. : E0988321C
Theoretical MW : 1661.99
Observed MW : 1662.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200
Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH