

Sample Name : Ghrelin, rat
 Cat. No. : RP10781
 Lot. No. : PE4841611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

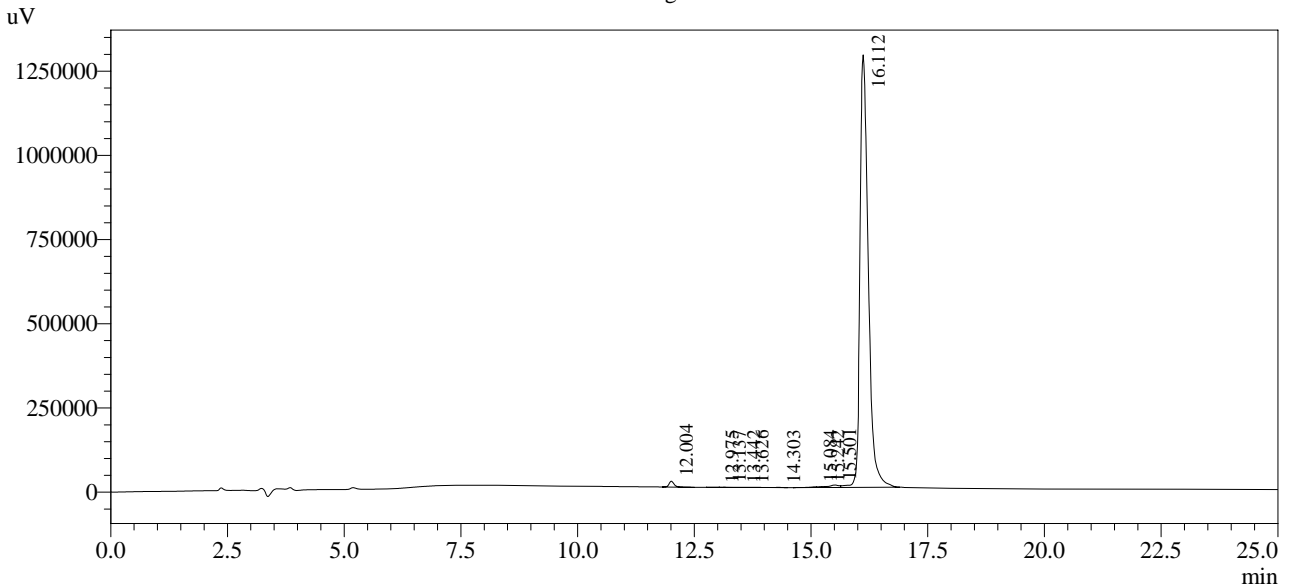

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.004	131924	17414	0.812
2	12.975	3110	268	0.019
3	13.137	7314	457	0.045
4	13.442	3482	332	0.021
5	13.626	9469	478	0.058
6	14.303	5949	559	0.037
7	15.084	22331	2030	0.137
8	15.242	25809	2779	0.159
9	15.501	103523	7358	0.637
10	16.112	15929437	1284168	98.073
Total		16242347	1315843	100.000