

Sample Name:hgp100(25-33)
 Cat No. :RP20344
 Lot No. :E8898721F
 Time Processed :20:27:03
 Month-Day-Year Processed :06/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

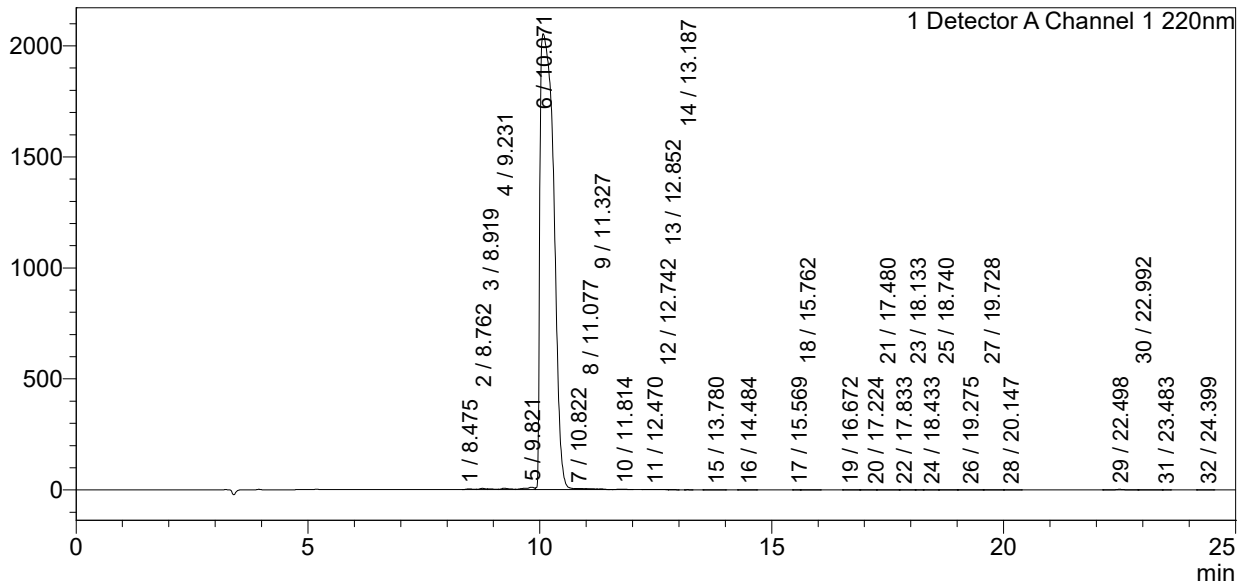

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.475	31429	3043	0.074
2	8.762	50778	5370	0.119
3	8.919	29325	2902	0.069
4	9.231	75266	6251	0.176
5	9.821	149333	10838	0.350
6	10.071	42143128	2053862	98.794
7	10.822	7352	979	0.017
8	11.077	7913	1102	0.019
9	11.327	10263	1558	0.024
10	11.814	25887	1898	0.061
11	12.470	15699	882	0.037
12	12.742	2062	526	0.005
13	12.852	7048	1164	0.017
14	13.187	1117	243	0.003

Peak#	Ret. Time	Area	Height	Area%
15	13.780	2054	143	0.005
16	14.484	3352	417	0.008
17	15.569	1032	135	0.002
18	15.762	2602	176	0.006
19	16.672	5235	443	0.012
20	17.224	5639	374	0.013
21	17.480	11946	443	0.028
22	17.833	6448	373	0.015
23	18.133	2183	246	0.005
24	18.433	3458	227	0.008
25	18.740	2311	169	0.005
26	19.275	3732	235	0.009
27	19.728	1413	107	0.003
28	20.147	1387	144	0.003
29	22.498	36982	2695	0.087
30	22.992	8599	423	0.020
31	23.483	1135	122	0.003
32	24.399	1398	116	0.003
Total		42657508	2097606	100.000