

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No. :RP11529
 Lot No. :E4744219I
 Time Processed :8:56:16
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

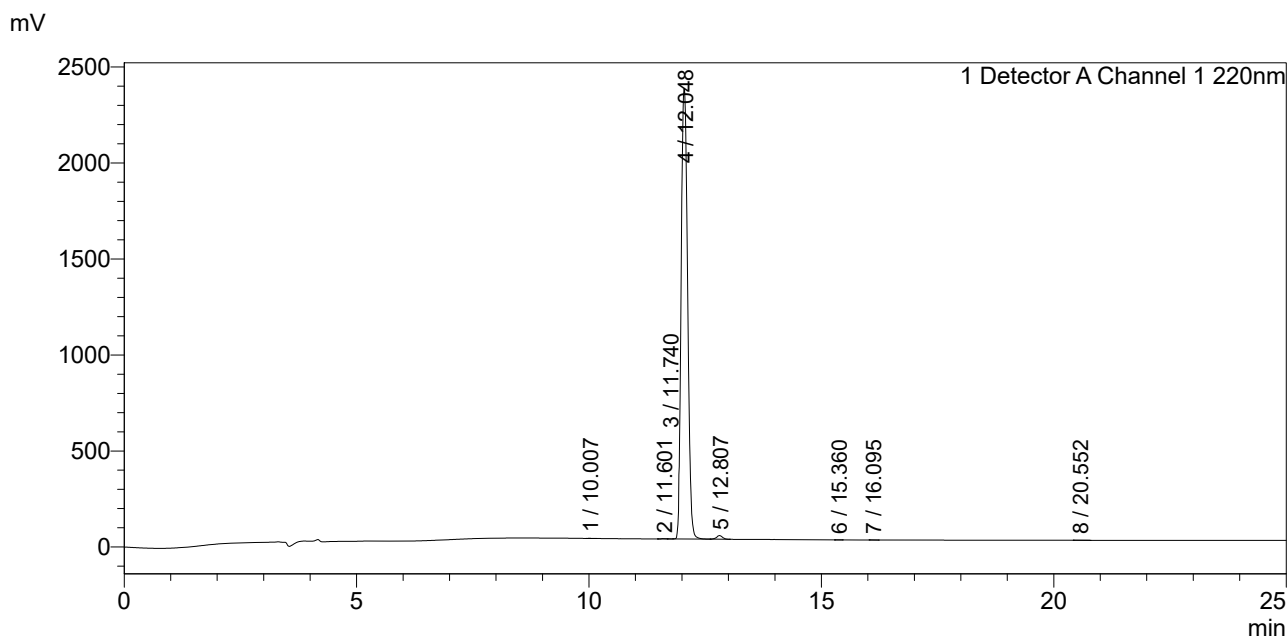

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.007	2349	411	0.010
2	11.601	11310	1874	0.050
3	11.740	7318	1263	0.032
4	12.048	22613800	2346401	99.132
5	12.807	168161	19009	0.737
6	15.360	1818	357	0.008
7	16.095	1345	268	0.006
8	20.552	5627	745	0.025
Total		22811727	2370329	100.000