

Sample Name :DYKDDDDK Peptide
 Cat No. :RP10586
 Lot No. :E8621420L
 Time Processed :9:58:00 AM
 Month-Day-Year Processed :12/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	0
25.00	Pumps	B.Conc	50
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

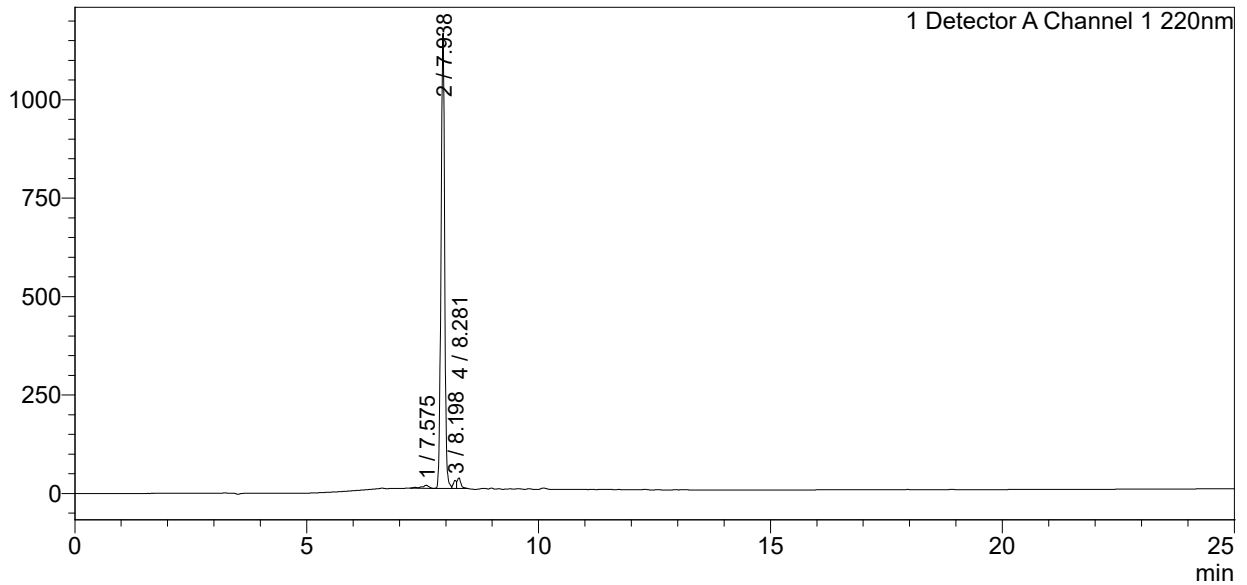

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.575	83585	7773	1.275
2	7.938	6233813	1156281	95.105
3	8.198	96308	20334	1.469
4	8.281	140987	26699	2.151
Total		6554693	1211088	100.000