

Sample Name :Influenza A NP(366-374) Strain A/PR/8/35  
 Cat No. :RP20267  
 Lot No. :E9508220G  
 Time Processed :17:24:24  
 Month-Day-Year Processed :08/02/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

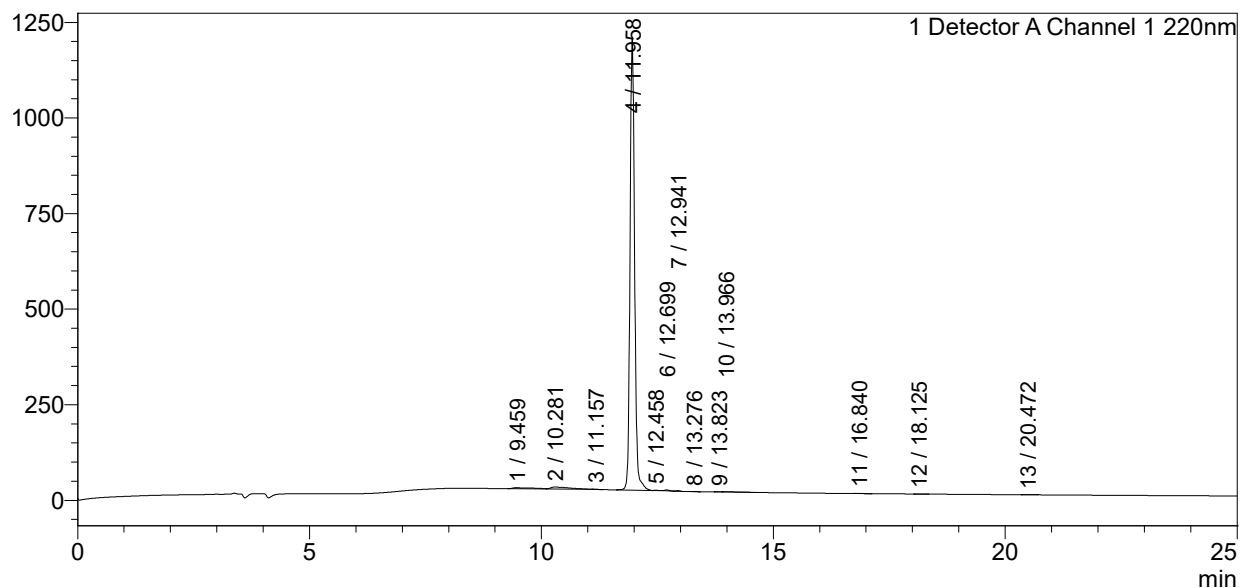

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.459	95253	2868	1.127
2	10.281	147985	5222	1.751
3	11.157	2444	523	0.029
4	11.958	8155824	1179805	96.479
5	12.458	4299	965	0.051
6	12.699	15643	2365	0.185
7	12.941	9837	1741	0.116
8	13.276	3289	487	0.039
9	13.823	2410	309	0.029
10	13.966	10863	540	0.129
11	16.840	1126	128	0.013
12	18.125	1010	142	0.012
13	20.472	3528	413	0.042
Total		8453513	1195508	100.000