

Sample Name: GRGDSPC  
 Cat No. : RP20283  
 Lot No. : E3429120B  
 Time Processed: 10:45:05 AM  
 Month-Day-Year Processed :02/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

<Chromatogram>

mV

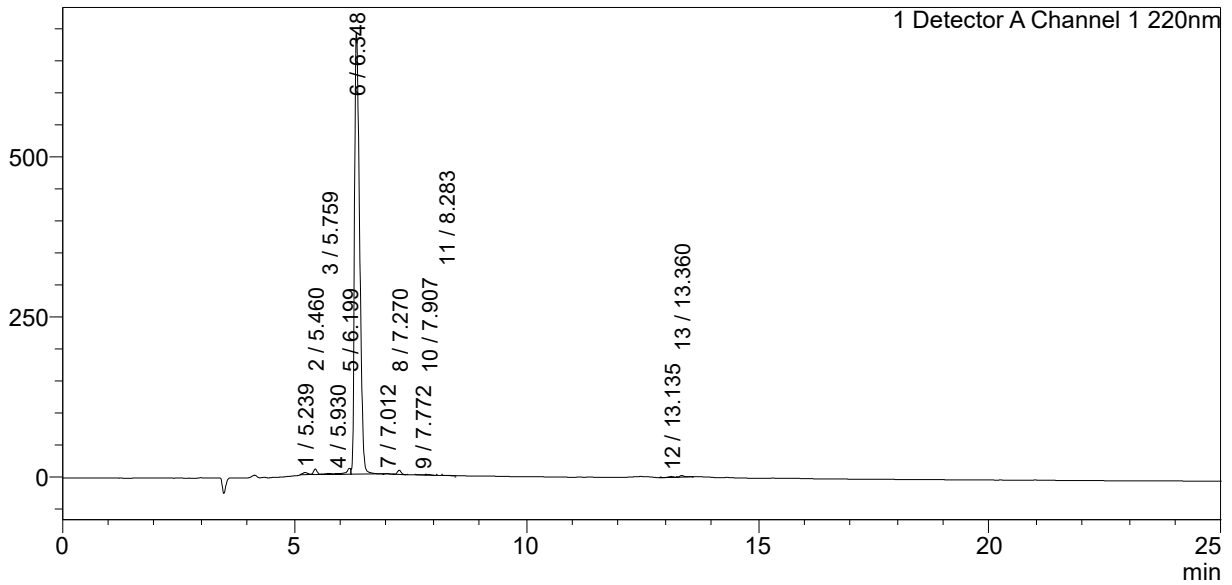

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.239	24785	3274	0.449
2	5.460	46846	8631	0.849
3	5.759	15753	1378	0.285
4	5.930	9061	1251	0.164
5	6.199	63071	9373	1.143
6	6.348	5278776	690145	95.640
7	7.012	4248	789	0.077
8	7.270	35614	6703	0.645
9	7.772	2716	398	0.049
10	7.907	5973	1025	0.108
11	8.283	2443	372	0.044
12	13.135	11877	1463	0.215
13	13.360	18274	2575	0.331
Total		5519437	727376	100.000