


MS Spectrum Graph

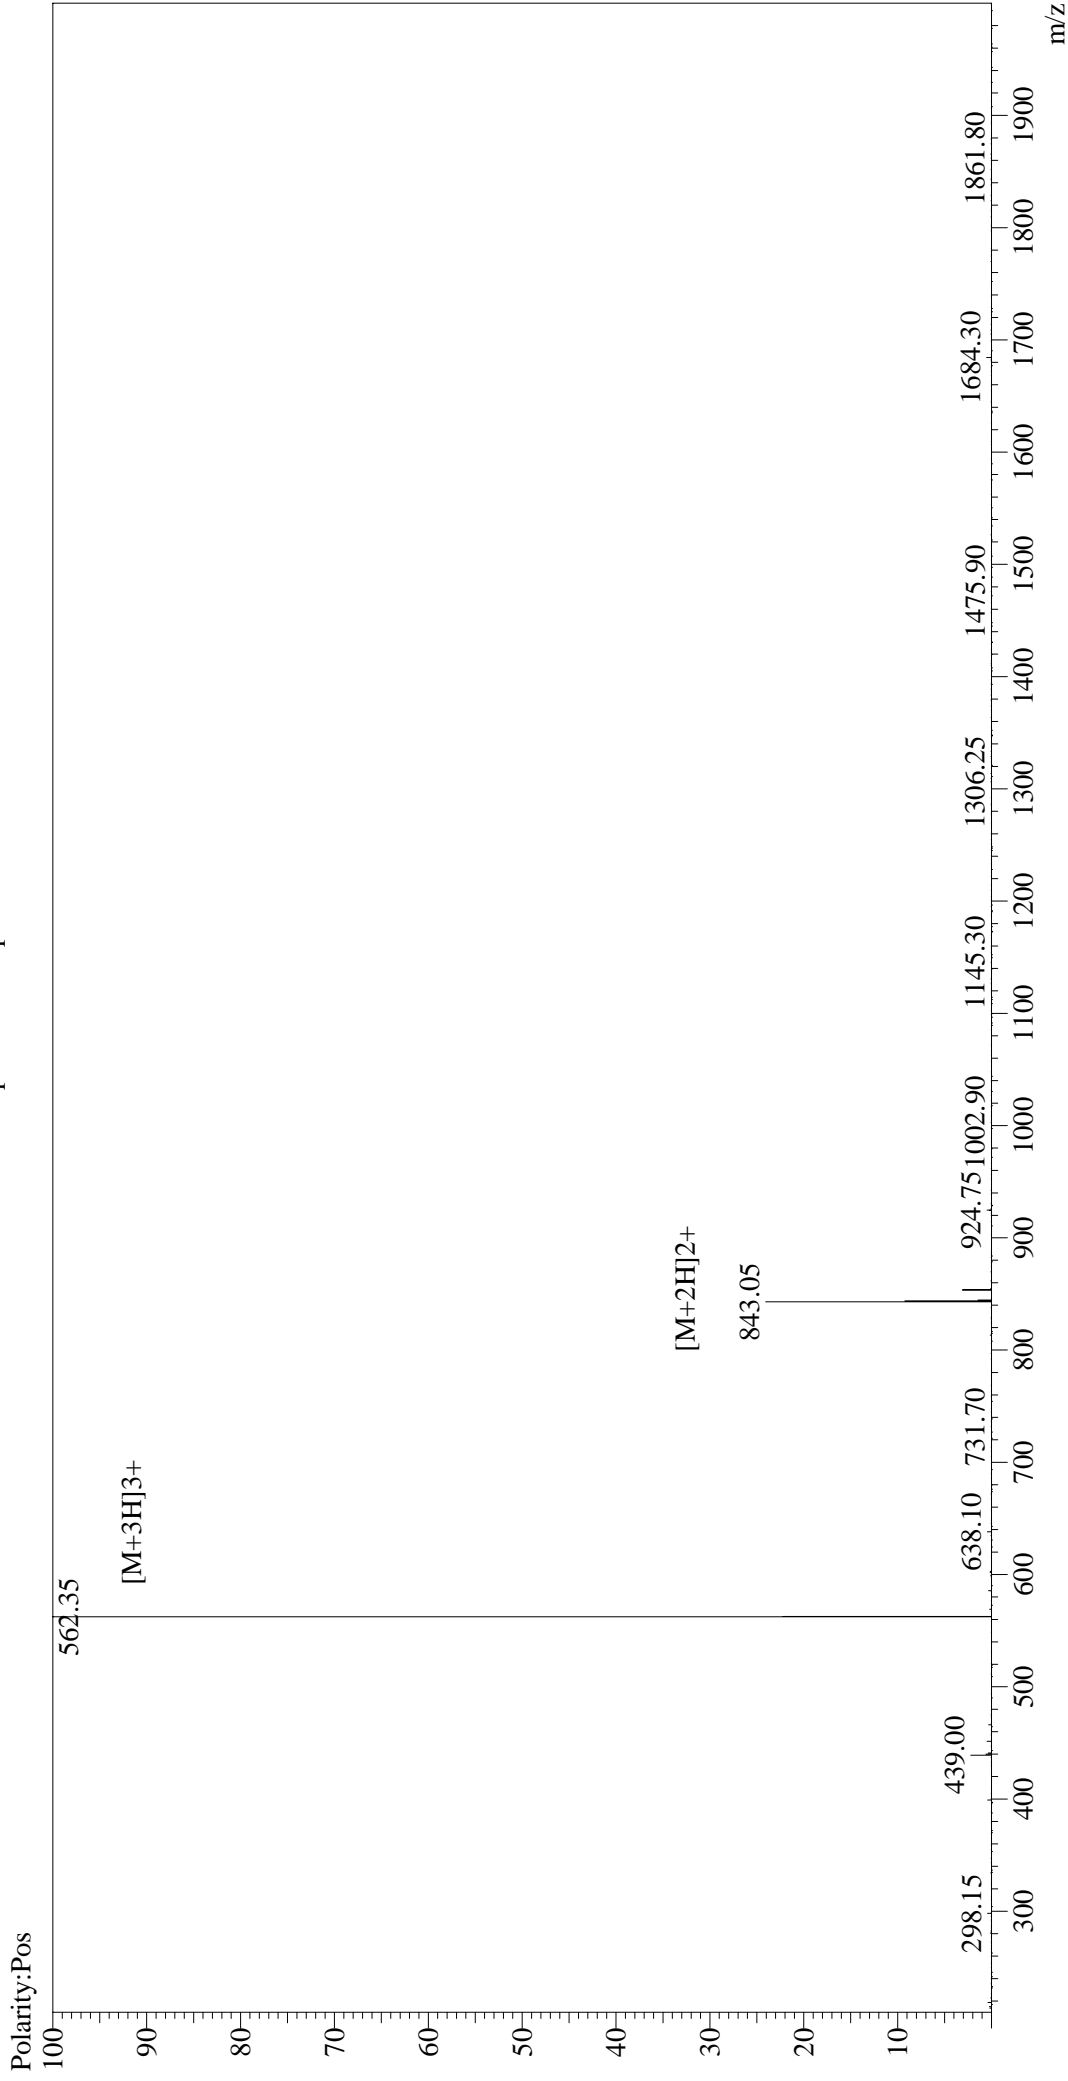

Sample Information
 Acquired by : Admin
 Date Acquired : 2016-12-23 9:42:43
 Injection Volume : 1
 Sample Name : a-Factor Mating Pheromone, yeast
 Cat No. : RP01002
 Lot No. : PE2561612
 Theoretical MW : 1683.98
 Observed MW : 1684.05

Interface :ESI
 Nebulizing Gas Flow :1.5L/min
 CDL Temp :250°C
 Block Temp :200°C
 Interface Bias : +4.5 kV
 Drying Gas Flow :5 L/min
 T.Flow :0.2 ml/min
 B.conc :50%H2O/50%MeOH