

Sample Name:β-Amyloid (1-40)
 Cat No:RP10004
 Lot No :E8096821C
 Time Processed :8:38:44 AM
 Month-Day-Year Processed :05/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 31.00 | Pumps | Pump A B.Conc | 95 |
| 31.01 | Pumps | Pump A B.Conc | 5 |
| 40.00 | Pumps | Pump A B.Conc | 5 |
| 40.01 | Controller | Stop | |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

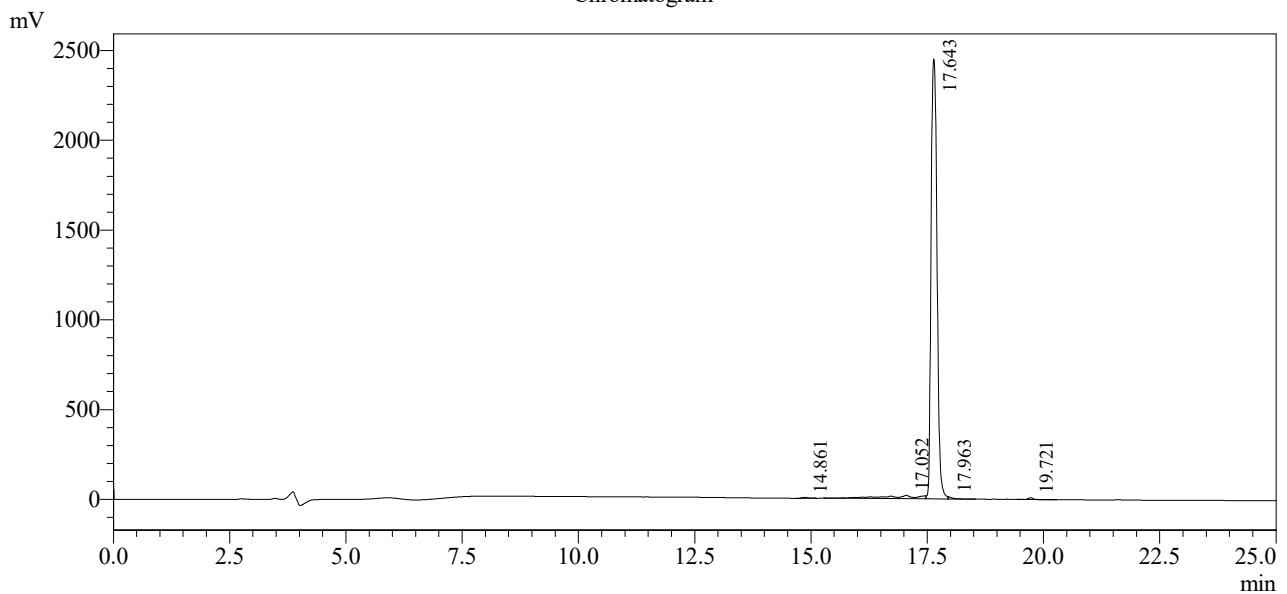

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|----------|---------|---------|
| 1 | 14.861 | 44253 | 5213 | 0.193 |
| 2 | 17.052 | 948304 | 18557 | 4.142 |
| 3 | 17.643 | 21758940 | 2450713 | 95.043 |
| 4 | 17.963 | 73468 | 11810 | 0.321 |
| 5 | 19.721 | 68927 | 9970 | 0.301 |
| Total | | 22893892 | 2496263 | 100.000 |