


Mass Spectrum

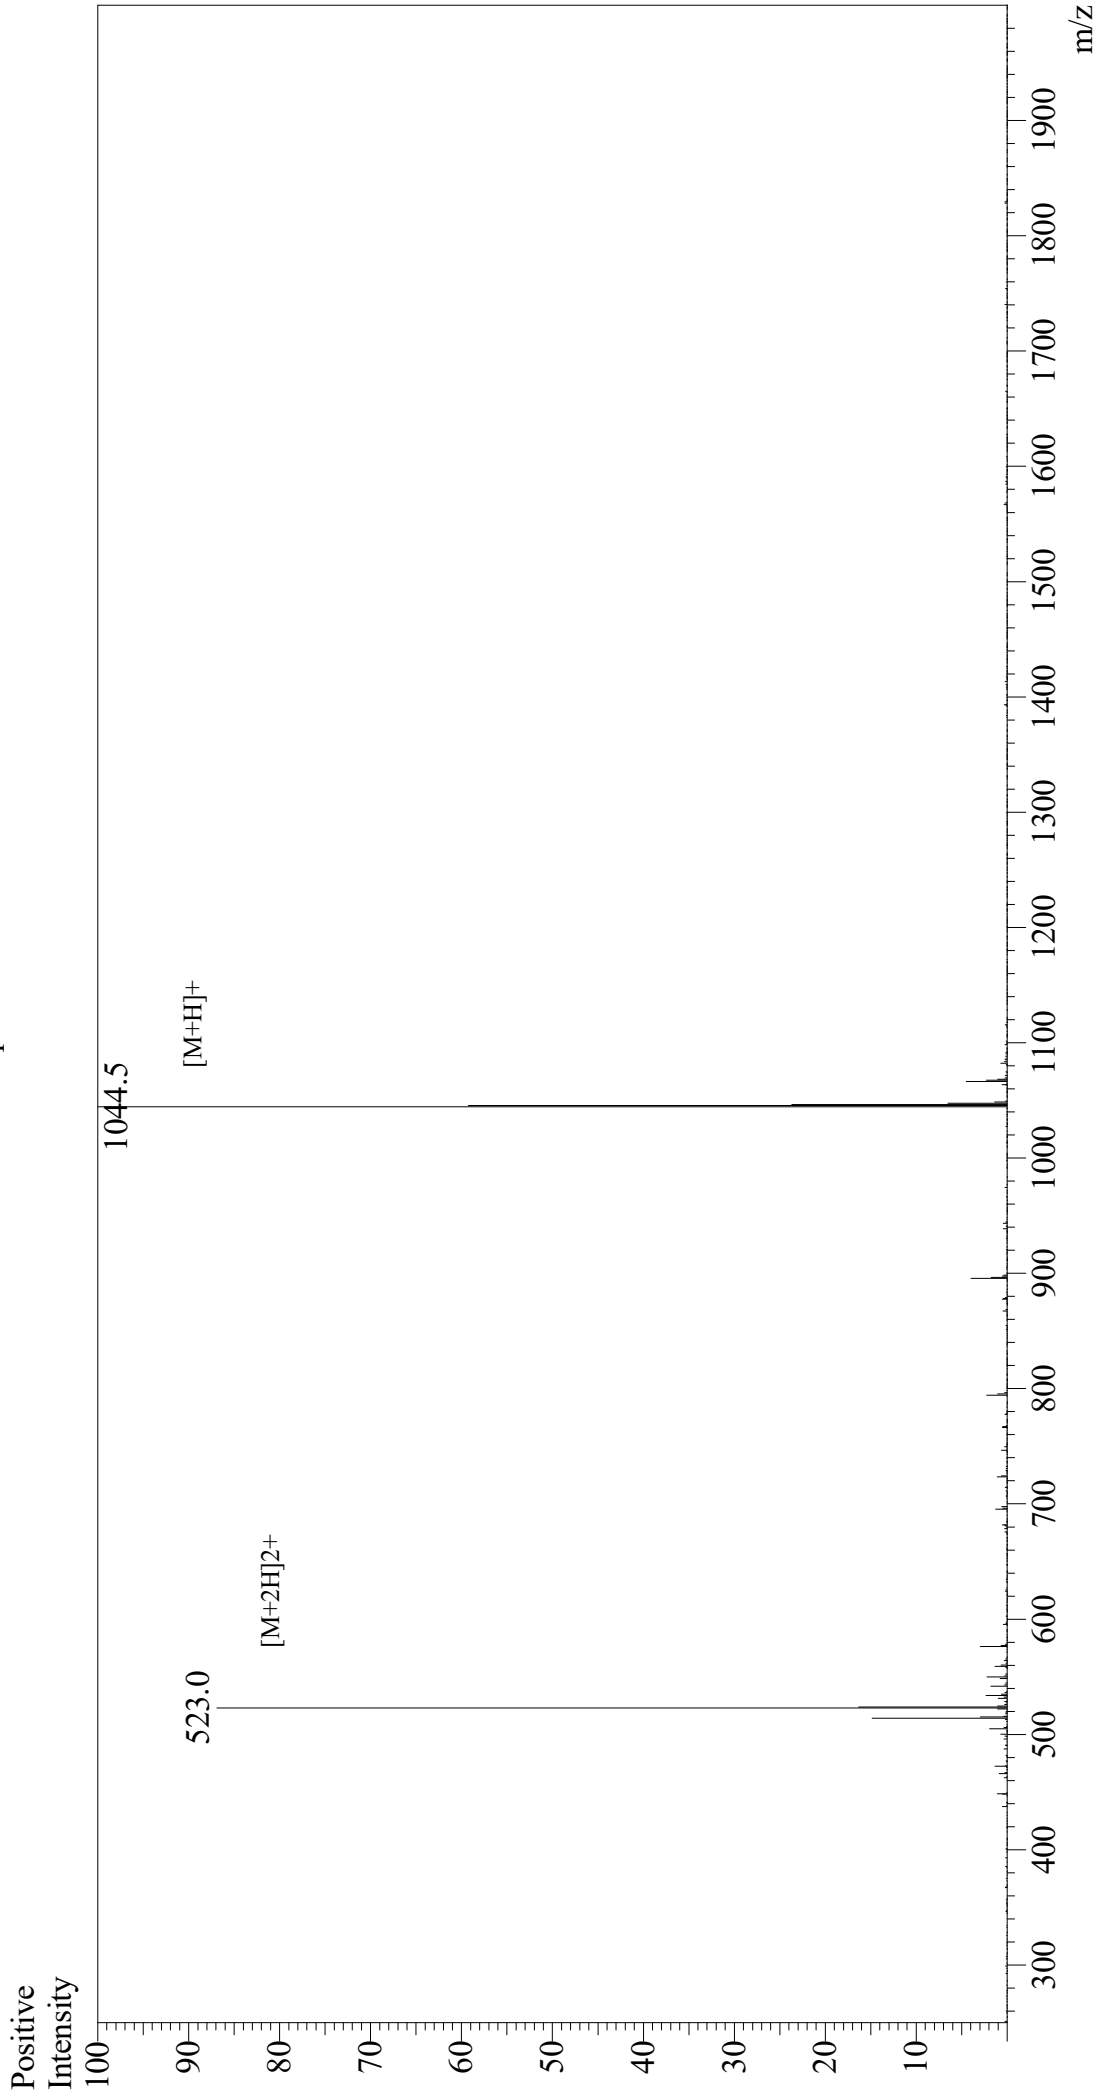

Sample Information

Month-Day Processed : 07/18/21
Time Processed : 7:08:54
Injection Volume : 0.2
Sample Name : LCMV gp33-41
Cat No. : RP20257
Lot No. : E1578321G
Theoretical MW : 1044.25
Observed MW : 1043.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH