

Sample Name : β -Amyloid (1-42), human
 Cat No. : RP20527
 Lot No. : PE9011902
 Time Processed : 14:28:13
 Month-Day-Year Processed : 03/21/2019

Pump A : 0.5% Ammonia solution in 100% water (v/v)
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment : SS-CM-0310

Chromatogram

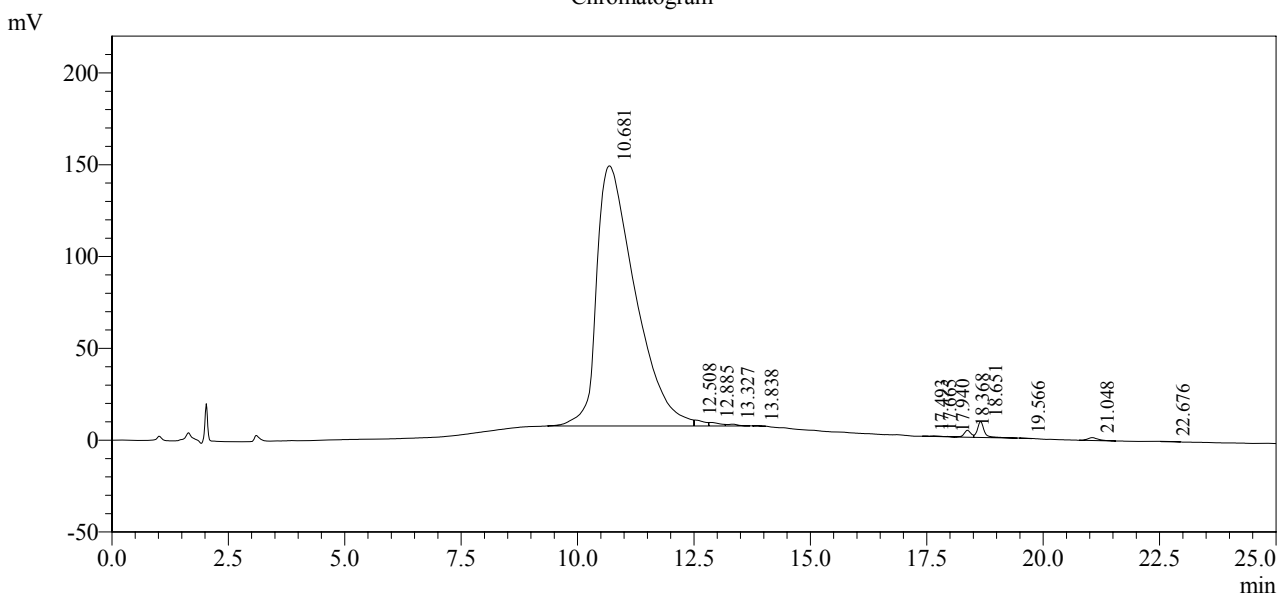

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.681	8154272	141673	96.901
2	12.508	48789	3255	0.580
3	12.885	31318	1935	0.372
4	13.327	16774	1012	0.199
5	13.838	1361	190	0.016
6	17.493	982	175	0.012
7	17.665	4149	395	0.049
8	17.940	1366	183	0.016
9	18.368	38064	3765	0.452
10	18.651	89015	8672	1.058
11	19.566	1141	132	0.014
12	21.048	24176	1549	0.287
13	22.676	3680	294	0.044
Total		8415087	163229	100.000