

Sample Name:Gastric Inhibitory Peptide (GIP), human
 Cat No. :RP10795
 Lot No. E3607620C
 Time Processed: 1:01:09 PM
 Month-Day-Year Processed :03/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

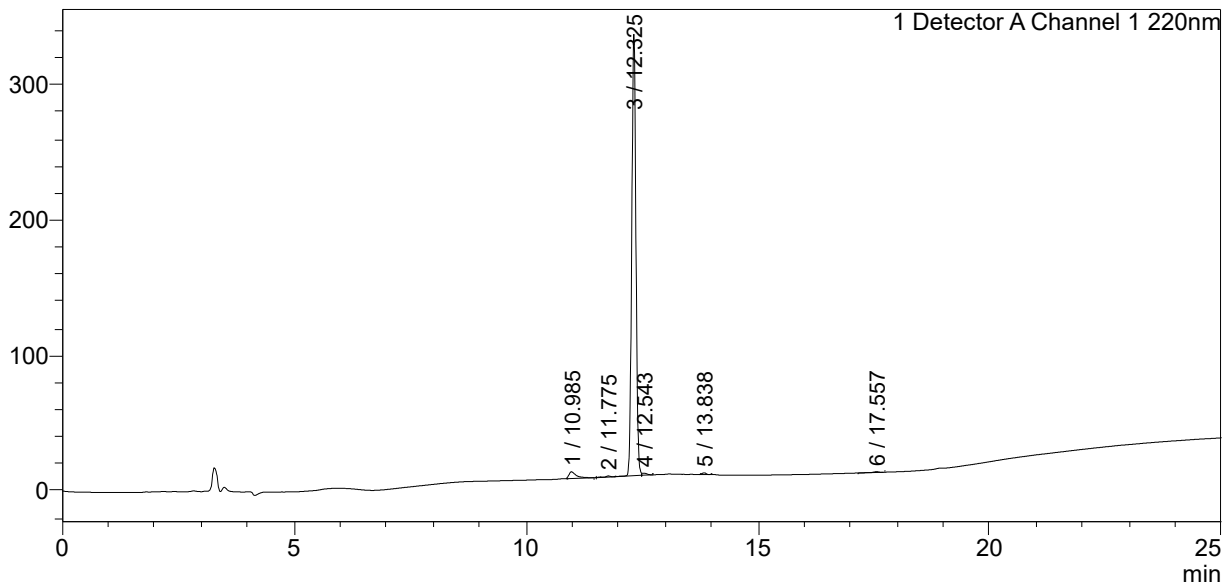

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.985	53591	4808	2.521
2	11.775	6971	719	0.328
3	12.325	2042503	318519	96.087
4	12.543	9974	1471	0.469
5	13.838	7876	1218	0.371
6	17.557	4767	575	0.224
Total		2125683	327309	100.000