

Sample Name :HA Peptide
 Cat No :RP11735
 Lot No :E6499121B
 Time Processed :10:14:30
 Month-Day-Year Processed :02/14/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

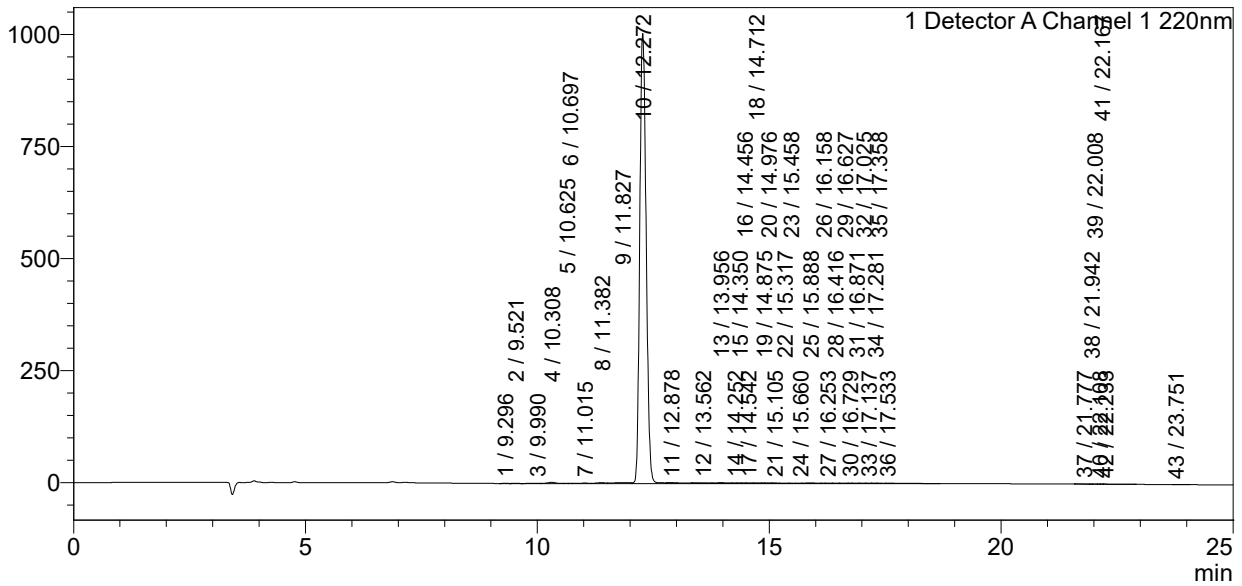

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.296	1891	239	0.019
2	9.521	2241	249	0.022
3	9.990	7986	608	0.080
4	10.308	33921	2609	0.340
5	10.625	1604	278	0.016
6	10.697	1308	289	0.013
7	11.015	14827	906	0.149
8	11.382	27364	1990	0.274
9	11.827	52338	1999	0.524
10	12.272	9737117	1004585	97.530
11	12.878	3455	471	0.035
12	13.562	7367	567	0.074
13	13.956	14827	1016	0.149
14	14.252	2540	409	0.025
15	14.350	2102	398	0.021
16	14.456	2264	385	0.023

Peak#	Ret. Time	Area	Height	Area%
17	14.542	3576	393	0.036
18	14.712	2980	326	0.030
19	14.875	1289	294	0.013
20	14.976	2786	313	0.028
21	15.105	2218	289	0.022
22	15.317	2940	249	0.029
23	15.458	1111	258	0.011
24	15.660	2642	326	0.026
25	15.888	9776	539	0.098
26	16.158	1338	270	0.013
27	16.253	2621	295	0.026
28	16.416	2402	278	0.024
29	16.627	3037	295	0.030
30	16.729	1292	285	0.013
31	16.871	2337	279	0.023
32	17.025	1883	237	0.019
33	17.137	1609	242	0.016
34	17.281	1471	223	0.015
35	17.358	1254	233	0.013
36	17.533	1836	213	0.018
37	21.777	3386	231	0.034
38	21.942	1175	301	0.012
39	22.008	1864	319	0.019
40	22.108	1295	329	0.013
41	22.167	1195	345	0.012
42	22.233	9714	372	0.097
43	23.751	1582	132	0.016
Total		9983761	1024866	100.000