


Mass Spectrum

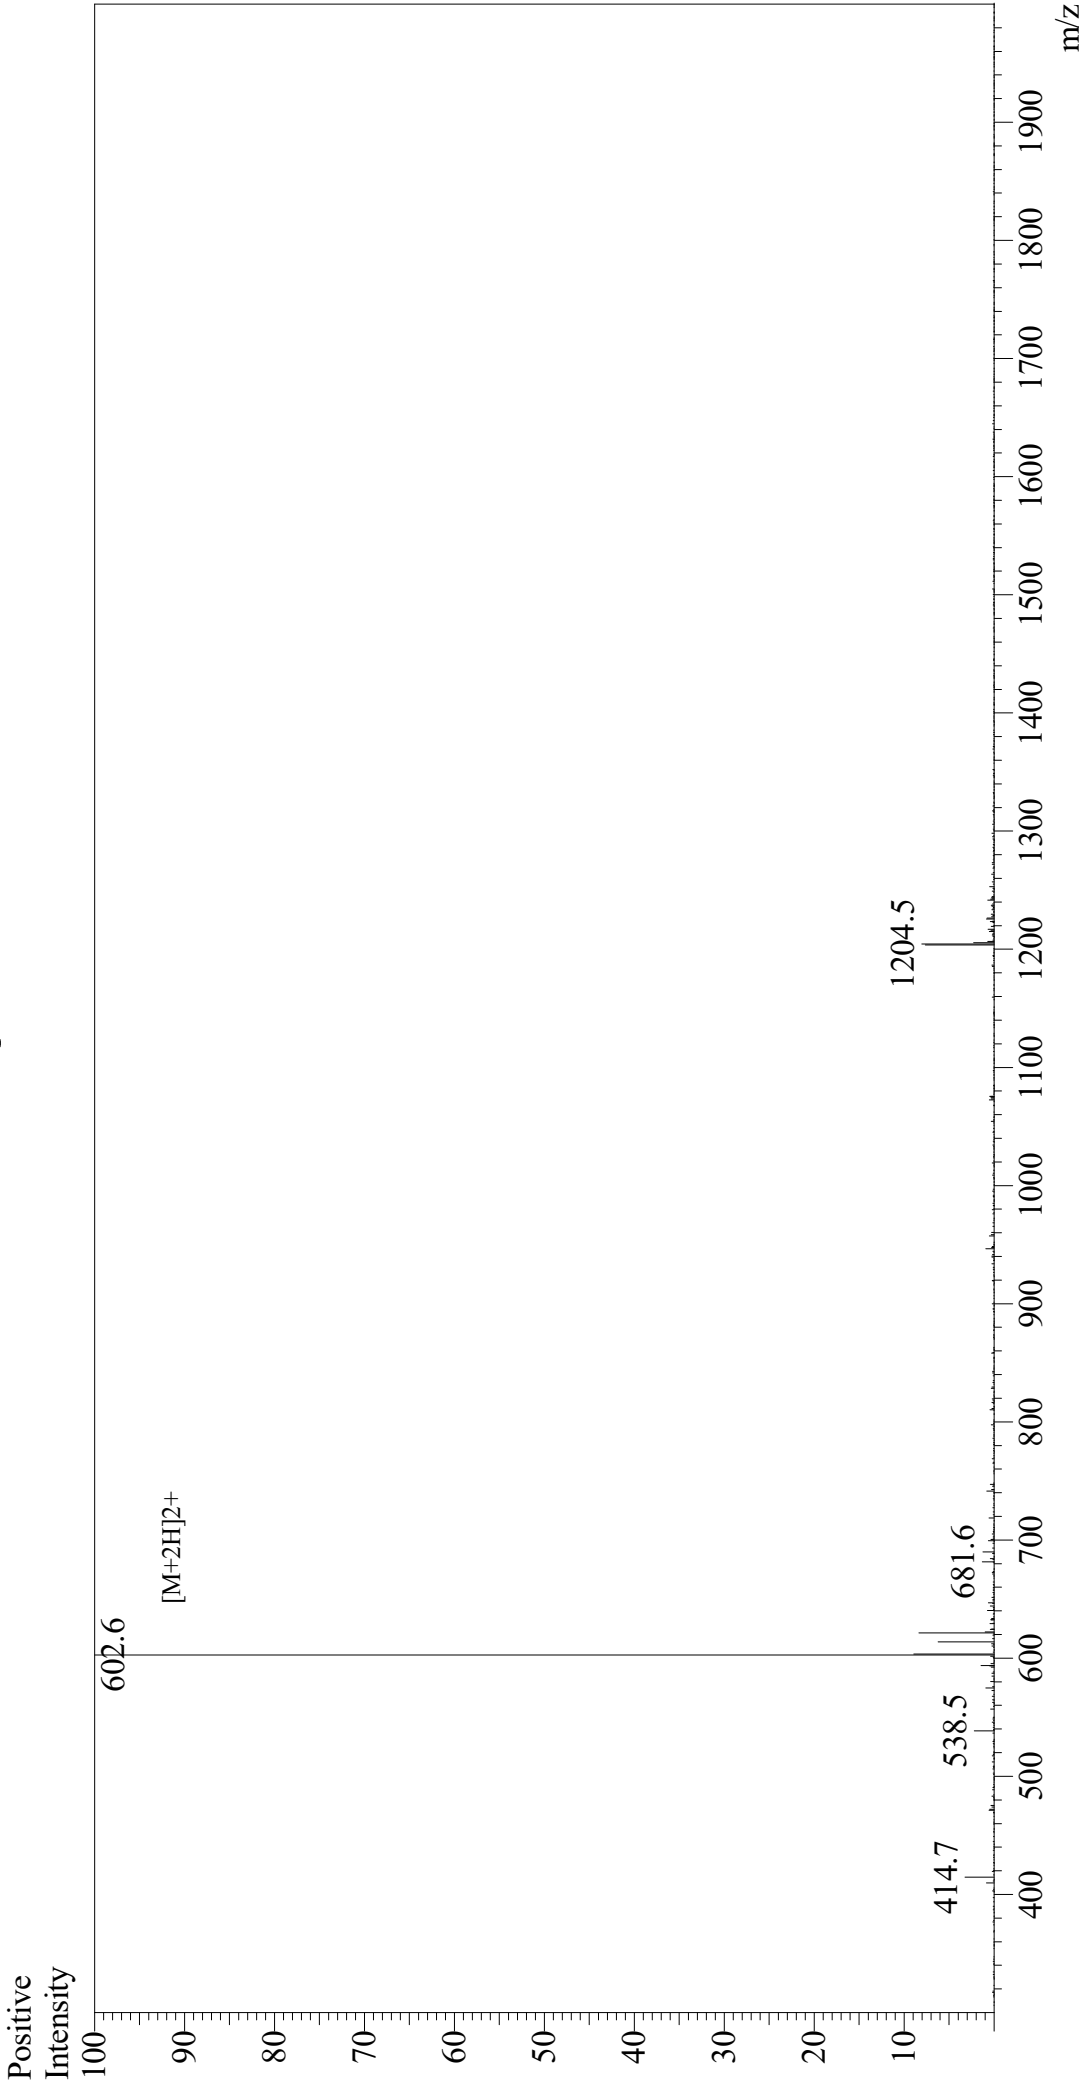

Sample Information

Acquired by: Gary
Month-Day Processed: 07/10/20
Time Processed: 12:15:43 PM
Injection Volume: 0.3
Sample Name: c-Myc Peptide
Cat No.: RPI1731
Lot No.: E7153020G
Theoretical MW: 1203.30
Observed MW: 1203.2

Interface: ESI
Nebulizing Gas Flow: 1.5L/min
CDL Temp: 250
Block Temp: 200

Equipment: GK11010007
Interface Bias: +4.5 kV
Drying Gas Flow: 5 L/min
T.Flow: 0.2 ml/min
B.conc: 50% H2O/50% MeOH