

Sample Name :OVA Peptide(257-264)  
 Cat No.: RP10611  
 Lot No. : PE2701708

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

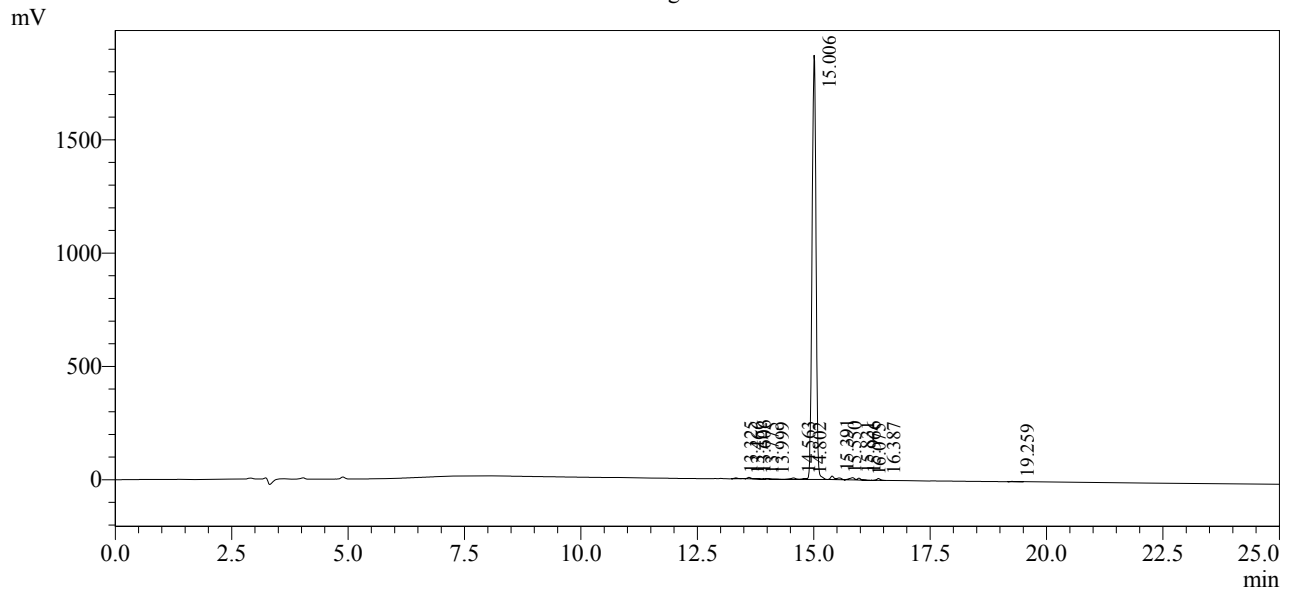

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.325	16970	3461	0.147
2	13.466	1543	459	0.013
3	13.606	34538	6395	0.299
4	13.775	8067	1674	0.070
5	13.999	20612	3362	0.178
6	14.563	57897	6649	0.501
7	14.802	29091	4488	0.252
8	15.006	11089885	1871294	96.001
9	15.391	75736	15346	0.656
10	15.550	48440	7450	0.419
11	15.831	73853	9801	0.639
12	15.966	41190	8081	0.357
13	16.075	3342	1178	0.029
14	16.387	42817	8103	0.371
15	19.259	7878	1472	0.068
Total		11551859	1949213	100.000