

Sample Name : OVA Peptide (257-264)  
 Cat. No. :RP10611  
 Lot. No. :PE7571902  
 Time Processed : 23:50:21  
 Month-Day-Year Processed : 02/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

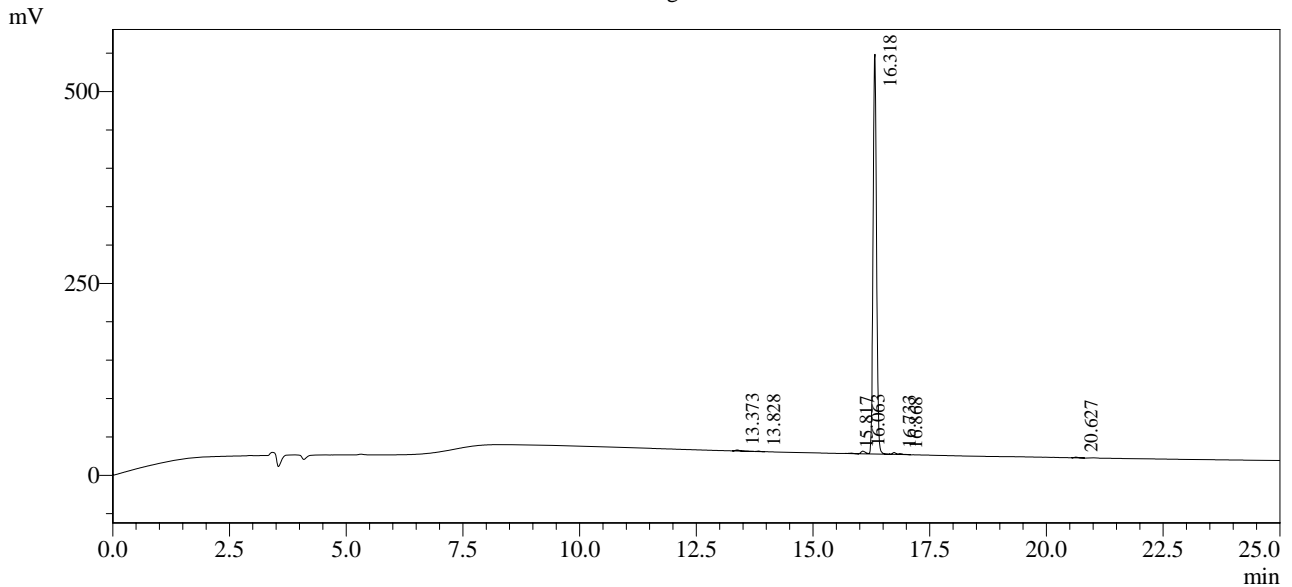

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.373	8100	1321	0.295
2	13.828	2775	609	0.101
3	15.817	3786	584	0.138
4	16.063	24008	3562	0.874
5	16.318	2684667	520901	97.721
6	16.733	12467	2384	0.454
7	16.868	6903	1225	0.251
8	20.627	4559	866	0.166
Total		2747266	531451	100.000