

Sample Name : β -Amyloid (1-40)
 Cat No.: RP10004
 Lot No.: E7090619K
 Time Processed : 13:19:39
 Month-Day-Year Processed : 12/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

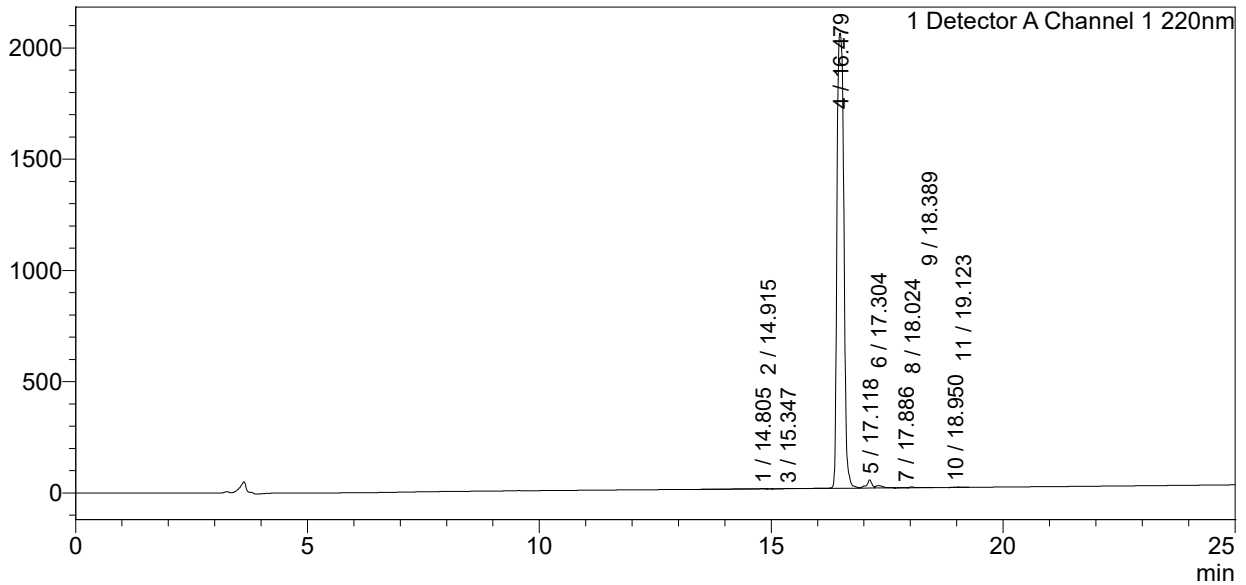

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.805	36632	2017	0.171
2	14.915	2468	579	0.012
3	15.347	4623	761	0.022
4	16.479	20921869	2046681	97.701
5	17.118	287539	36943	1.343
6	17.304	115165	10490	0.538
7	17.886	11719	1394	0.055
8	18.024	24073	3970	0.112
9	18.389	3194	546	0.015
10	18.950	1833	300	0.009
11	19.123	5005	841	0.023
Total		21414119	2104523	100.000