

Sample Name : hgp100(25-33)
 Cat. No. :RP20344
 Lot. No. :PE1791905
 Time Processed :9:36:32
 Month-Day-Year Processed :05/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

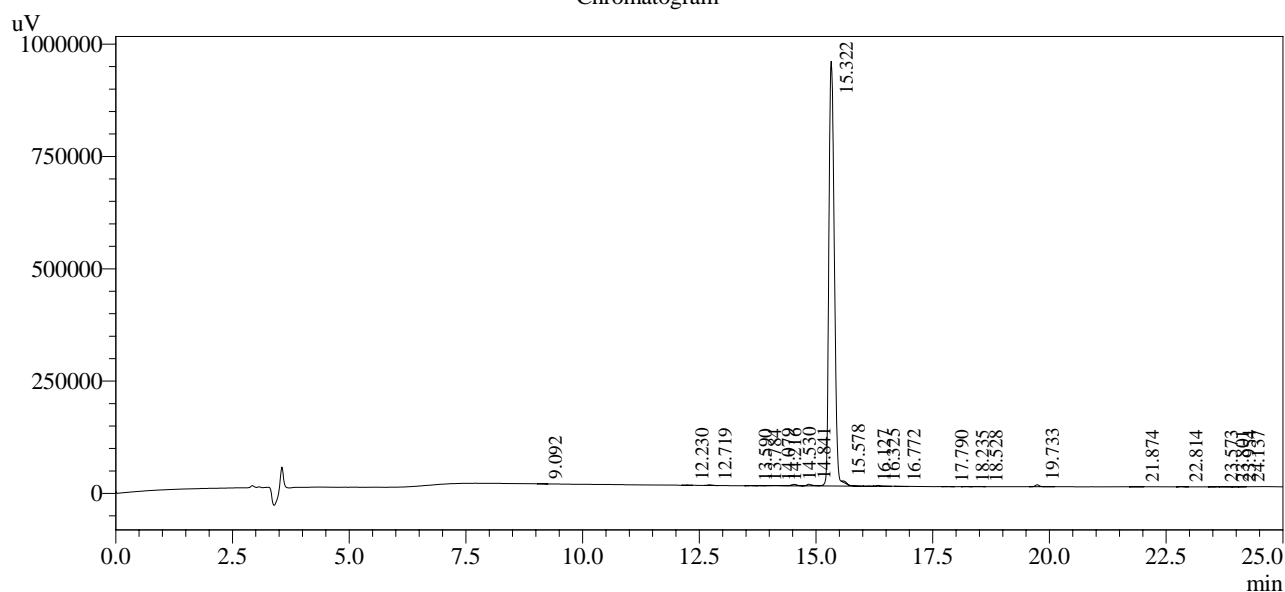

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.092	1693	312	0.022
2	12.230	1522	244	0.019
3	12.719	11461	1534	0.146
4	13.590	1625	204	0.021
5	13.784	1315	257	0.017
6	14.079	6986	1019	0.089
7	14.216	6257	1015	0.080
8	14.530	28977	3165	0.369
9	14.841	31655	3535	0.403
10	15.322	7674195	945558	97.719
11	15.578	17260	2465	0.220
12	16.127	2226	280	0.028
13	16.325	13641	1831	0.174
14	16.772	4745	725	0.060
15	17.790	1050	129	0.013
16	18.235	1204	153	0.015
17	18.528	2492	224	0.032
18	19.733	27764	4289	0.354
19	21.874	3112	315	0.040
20	22.814	6386	956	0.081
21	23.573	2188	246	0.028
22	23.801	2677	222	0.034
23	23.954	1455	235	0.019
24	24.137	1480	243	0.019

Peak#	Ret. Time	Area	Height	Area %
Total		7853368	969156	100.000