

Sample Name :SV40 T-Ag-derived NLS peptide
 Cat No: RP20513
 Lot No : E1073620J
 Time Processed :2:53:29 AM
 Month-Day-Year Processed :11/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

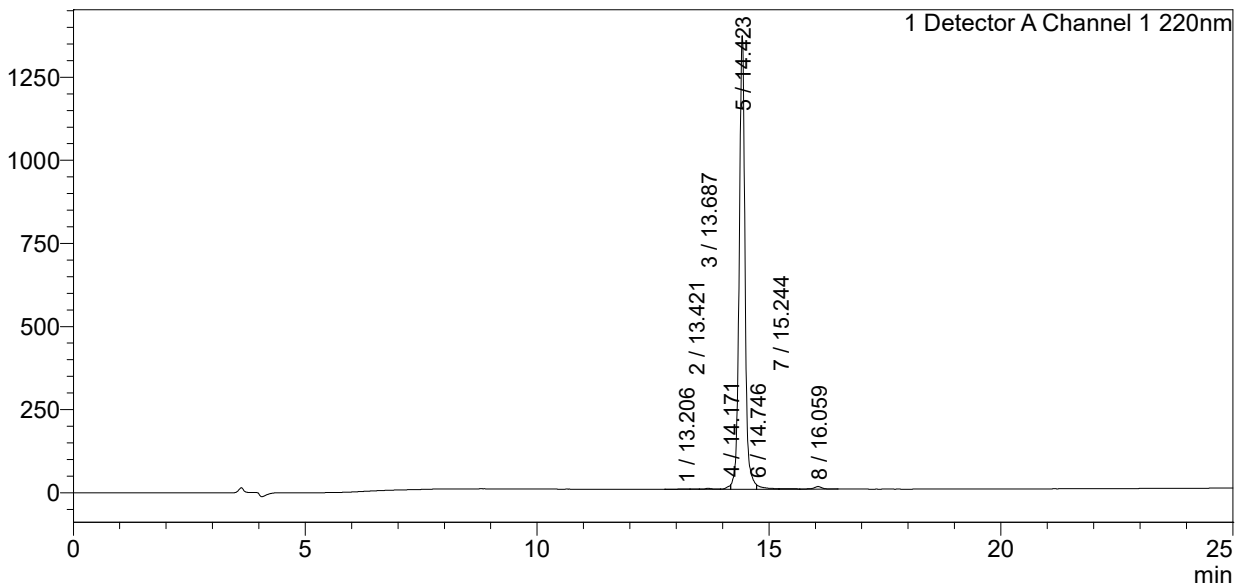

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.206	18157	1251	0.147
2	13.421	8835	782	0.072
3	13.687	39072	2941	0.317
4	14.171	65296	11517	0.530
5	14.423	11928836	1364940	96.830
6	14.746	122912	12452	0.998
7	15.244	35293	1599	0.286
8	16.059	100902	7830	0.819
Total		12319304	1403312	100.000