

Sample Name :TAT peptide
 Cat No.: RP20256
 Lot No.: E9002020G
 Time Processed :14:40:38
 Month-Day-Year Processed :07/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
33.00	Pumps	Solvent B Conc.	0
33.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

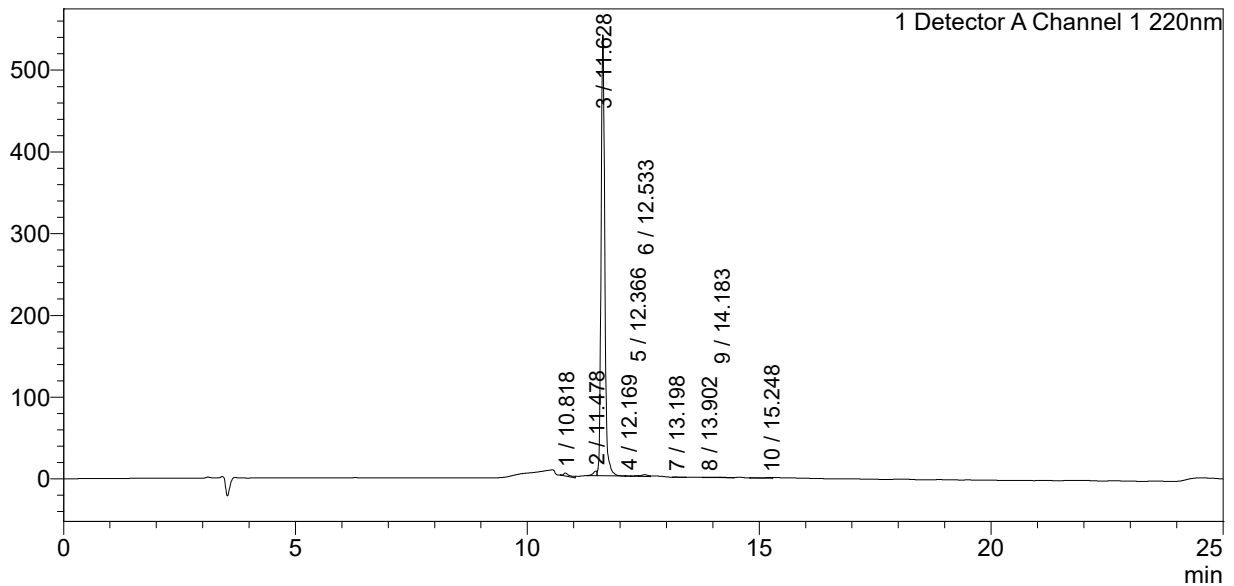

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.818	32575	3647	1.040
2	11.478	32174	5664	1.028
3	11.628	3005670	539637	96.003
4	12.169	1373	252	0.044
5	12.366	6522	899	0.208
6	12.533	24331	2373	0.777
7	13.198	1394	252	0.045
8	13.902	10412	491	0.333
9	14.183	6590	441	0.211
10	15.248	9767	578	0.312
Total		3130810	554233	100.000