

Sample Name : Melittin,honey bee
 Cat No. :RP20415
 Lot No. :PE5871702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
41.00	Pumps	Pump B Conc.	95
41.01	Pumps	Pump B Conc.	5
50.00	Pumps	Pump B Conc.	5
50.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

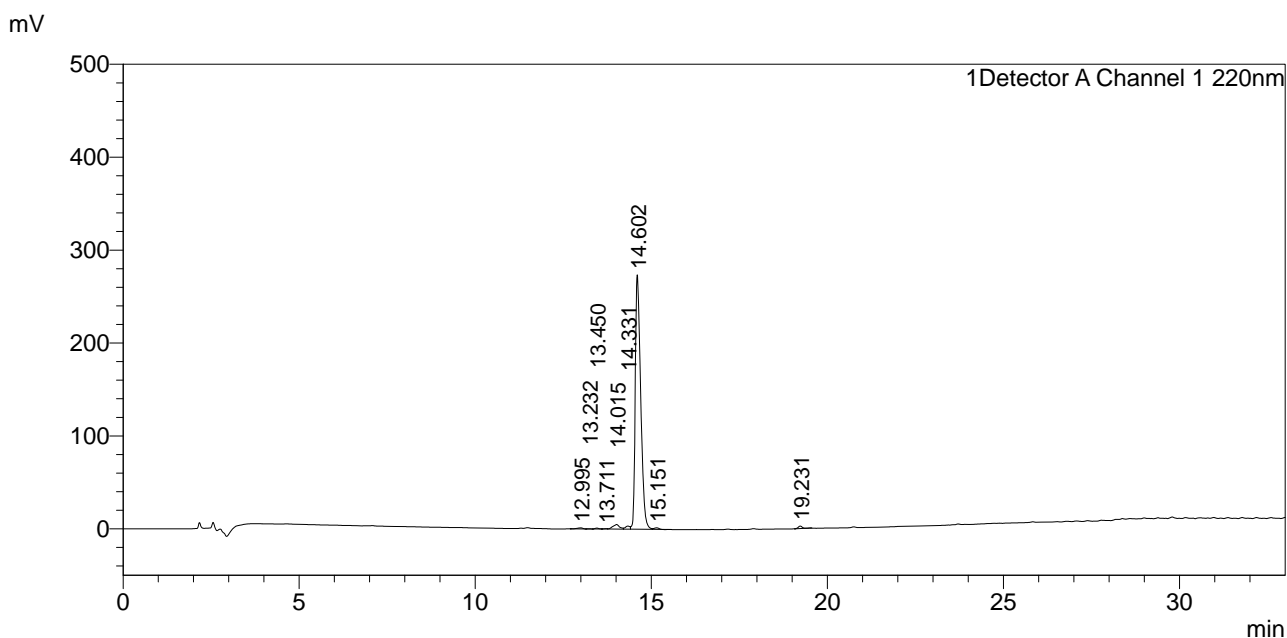

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.995	13020	1193	0.424
2	13.232	1163	183	0.038
3	13.450	6487	960	0.211
4	13.711	1298	187	0.042
5	14.015	63955	4900	2.082
6	14.331	29720	3347	0.967
7	14.602	2918657	273782	95.007
8	15.151	15485	1722	0.504
9	19.231	22272	2701	0.725
Total		3072057	288976	100.000