

Sample Information
 Sample Name :Hepatitis B Virus Core (128-140)
 Cat. No :RP17313
 Lot. No. :PE3411801

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
35.00	Pumps	Solvent B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

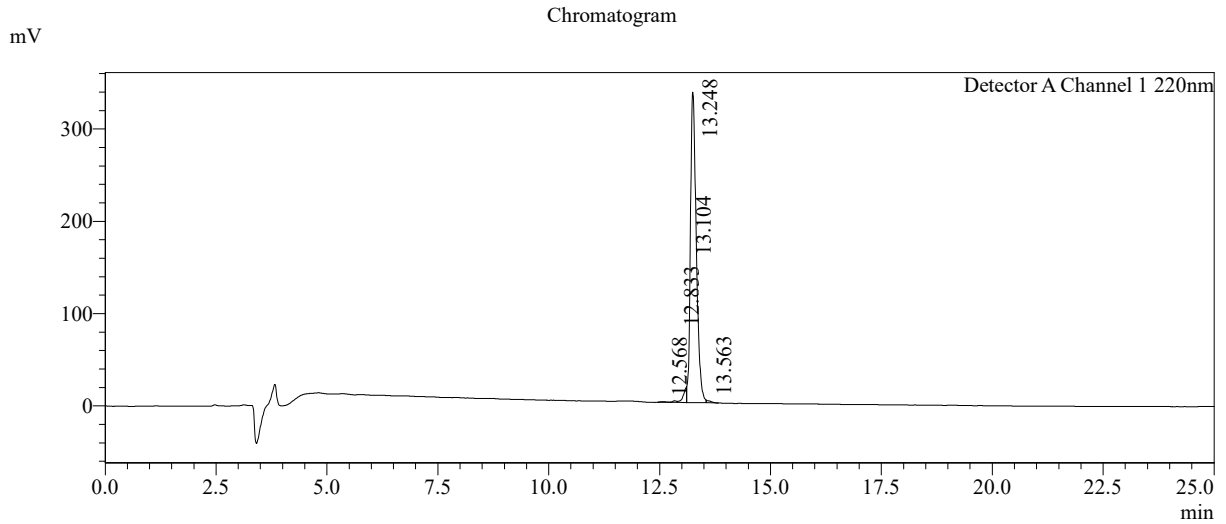

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	12.568	825	7524	0.231	0.235
2	12.833	1726	11230	0.482	0.351
3	13.104	16401	84127	4.584	2.628
4	13.248	336241	3081110	93.988	96.263
5	13.563	2556	16735	0.714	0.523
Total		357749	3200726	100.000	100.000