

Sample Name :MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E0789719G
 Time Processed : 21:44:35
 Month-Day-Year Processed : 07/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

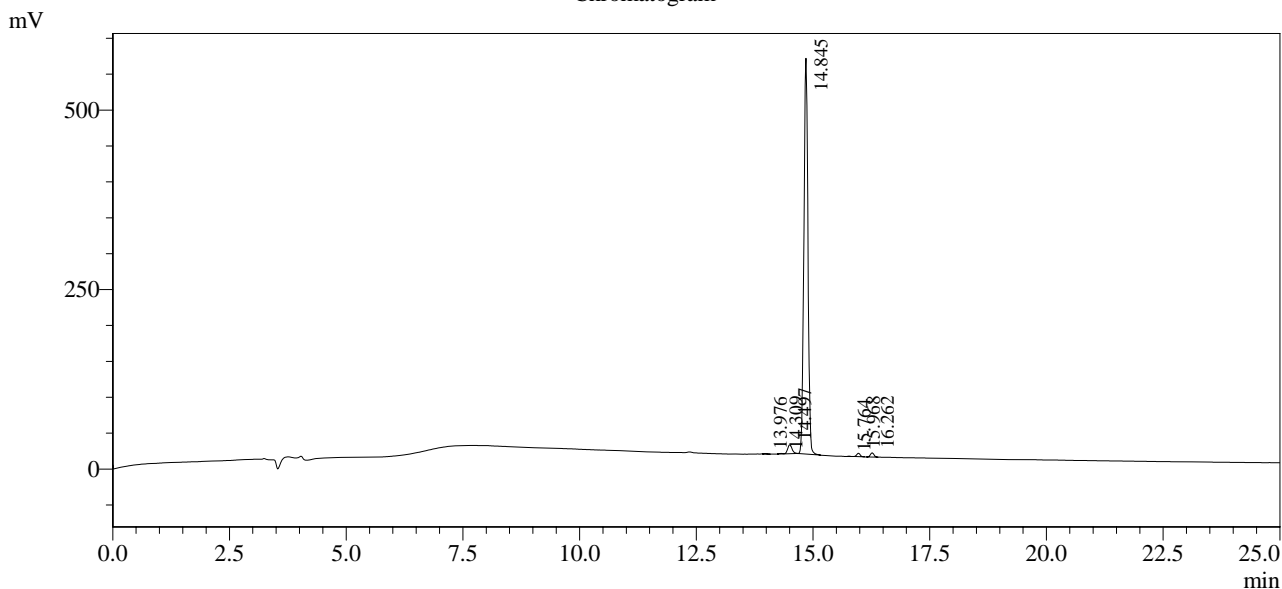

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.976	1282	280	0.037
2	14.309	4016	802	0.116
3	14.497	81202	12365	2.336
4	14.845	3334511	551322	95.934
5	15.764	845	360	0.024
6	15.968	23846	4732	0.686
7	16.262	30151	5823	0.867
Total		3475853	575684	100.000