

Sample Name :LAH4  
 Cat No :RP20096  
 Lot No :E1757321A  
 Time Processed :19:09:07  
 Month-Day-Year Processed :01/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010011

<Chromatogram>

mV

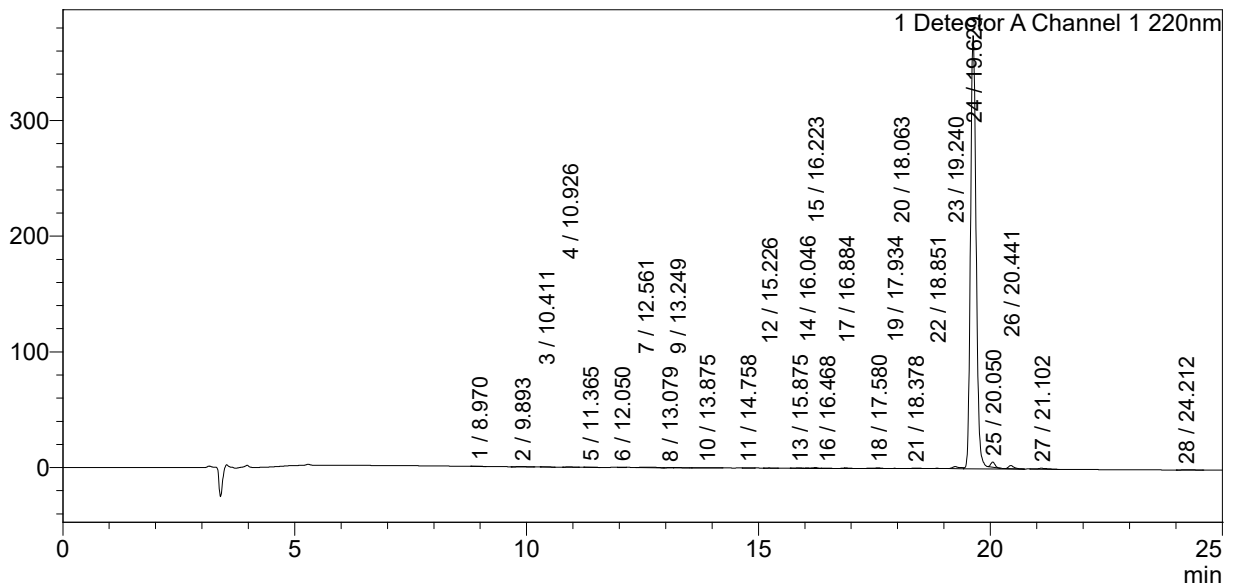

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.970	1157	123	0.035
2	9.893	2990	196	0.090
3	10.411	1090	110	0.033
4	10.926	2463	206	0.074
5	11.365	1480	119	0.044
6	12.050	1115	112	0.033
7	12.561	7671	377	0.230
8	13.079	1097	111	0.033
9	13.249	2287	180	0.069
10	13.875	3561	179	0.107
11	14.758	1874	153	0.056
12	15.226	1302	116	0.039
13	15.875	4156	358	0.125
14	16.046	2578	335	0.077
15	16.223	6024	706	0.181
16	16.468	2937	236	0.088

Peak#	Ret. Time	Area	Height	Area%
17	16.884	5467	457	0.164
18	17.580	7569	534	0.227
19	17.934	1359	170	0.041
20	18.063	1327	156	0.040
21	18.378	4164	276	0.125
22	18.851	2180	277	0.065
23	19.240	20737	1812	0.622
24	19.629	3180538	374507	95.472
25	20.050	27127	4497	0.814
26	20.441	21519	2705	0.646
27	21.102	12018	825	0.361
28	24.212	3578	295	0.107
Total		3331367	390128	100.000