

Sample Name : CEF20
 Cat. No. : RP11781
 Lot. No. : E6830220D
 Time Processed : 2:48:43
 Month-Day-Year Processed : 04/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

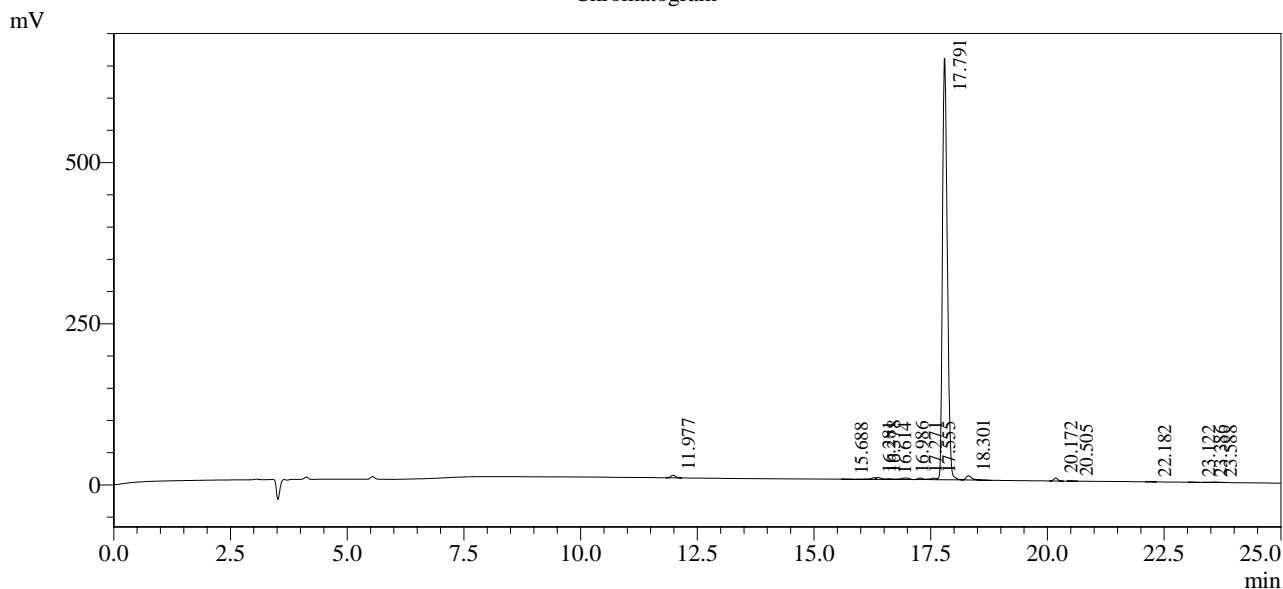

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.977	28686	4063	0.579
2	15.688	2271	359	0.046
3	16.281	20739	2643	0.418
4	16.378	22008	2994	0.444
5	16.614	6981	953	0.141
6	16.986	27812	2337	0.561
7	17.271	17590	2468	0.355
8	17.555	23057	2238	0.465
9	17.791	4709684	653820	95.031
10	18.301	56692	6493	1.144
11	20.172	27887	4642	0.563
12	20.505	1240	233	0.025
13	22.182	1010	159	0.020
14	23.122	1483	244	0.030
15	23.386	1933	305	0.039
16	23.588	6882	716	0.139
Total		4955956	684666	100.000