

Sample Name : Melittin,honey bee  
 Cat. No. : RP20415  
 Lot. No. : PE7461902  
 Time Processed : 17:47:09  
 Month-Day-Year Processed : 02/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

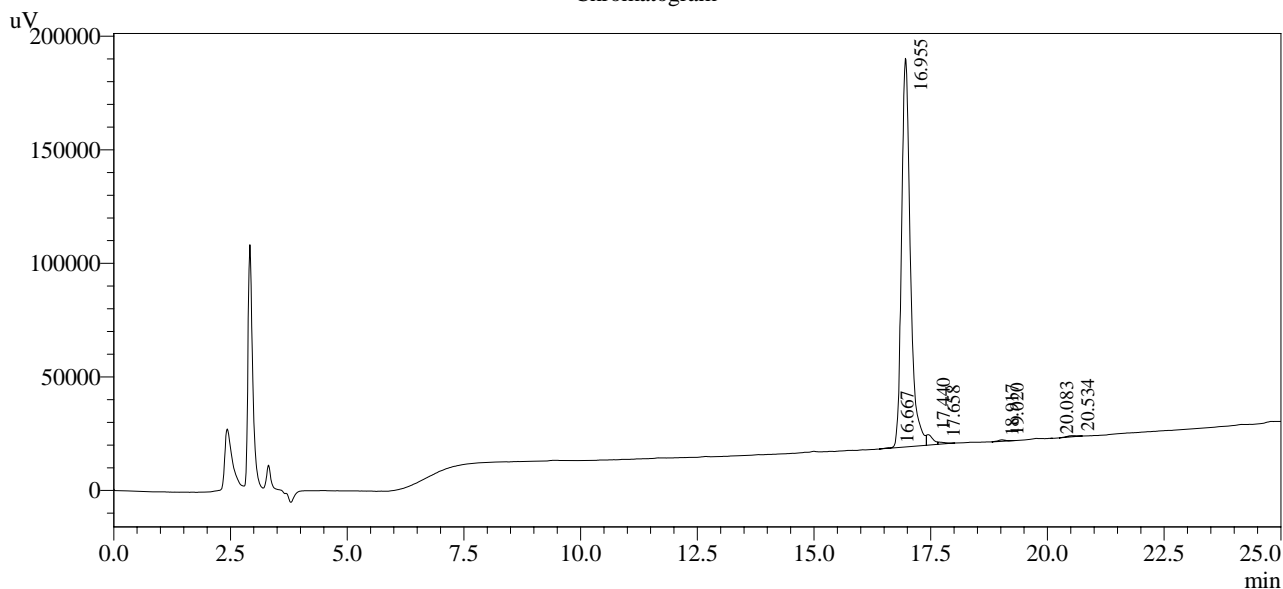

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.667	2018	202	0.087
2	16.955	2243206	171142	97.070
3	17.440	41631	4614	1.802
4	17.658	9477	1008	0.410
5	18.917	1023	221	0.044
6	19.020	6112	643	0.264
7	20.083	12	1	0.001
8	20.534	7446	494	0.322
Total		2310925	178325	100.000