

Sample Name :OVApeptide(323-339)  
 Cat. No. : RP10610  
 Lot. No. : PE3321904  
 Time Processed : 17:18:11  
 Month-Day-Year Processed : 04/22/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

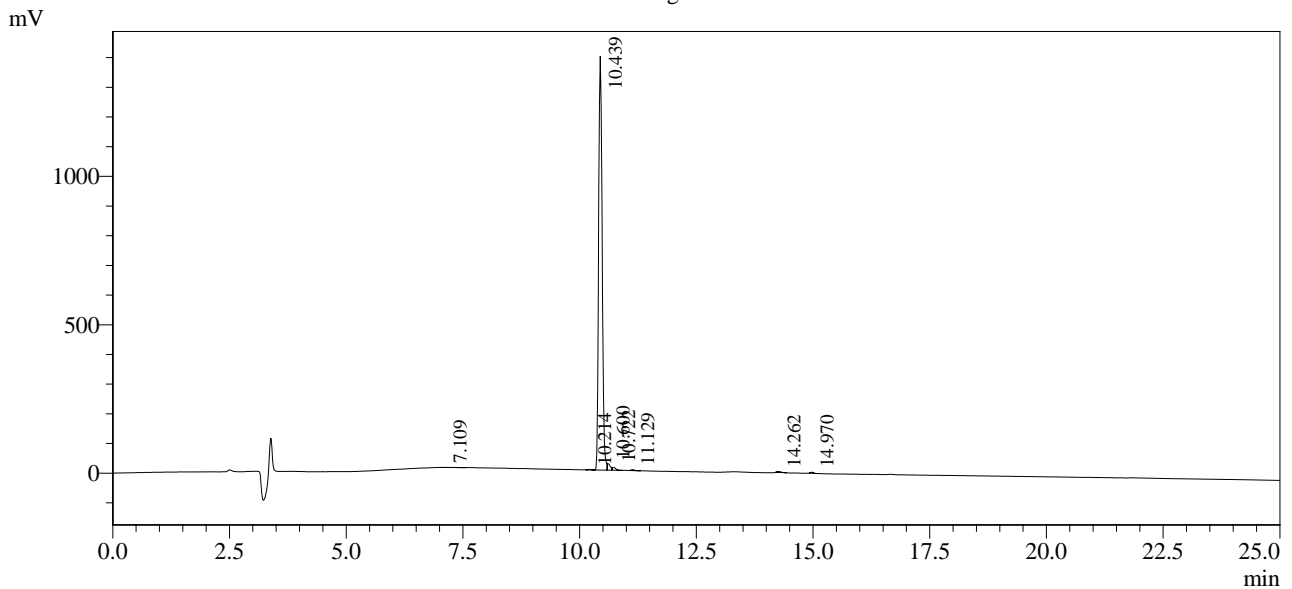

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.109	7453	347	0.098
2	10.214	6817	1556	0.090
3	10.439	7402964	1393991	97.277
4	10.600	94227	22409	1.238
5	10.722	49271	9603	0.647
6	11.129	15596	3129	0.205
7	14.262	18953	3076	0.249
8	14.970	14915	3469	0.196
Total		7610195	1437580	100.000