

Sample Name :LL37 (Human)
 Cat. No. : RP13323
 Lot. No. : E3585820B
 Time Processed :8:40:41
 Month-Day-Year Processed :02/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

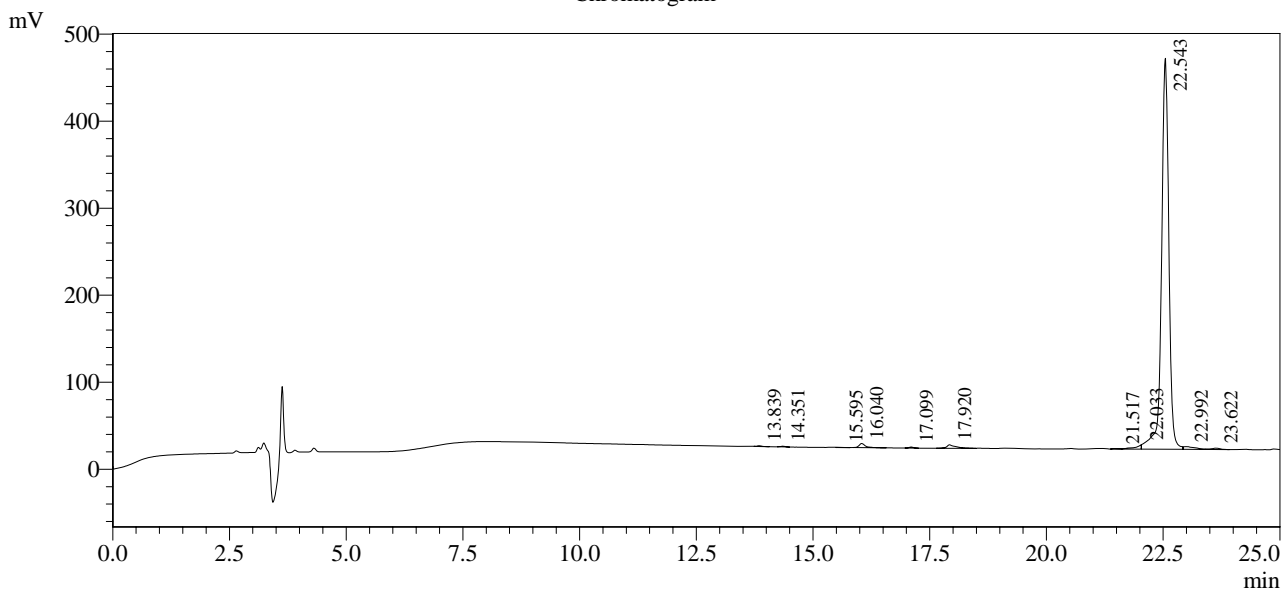

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.839	6572	973	0.127
2	14.351	4218	704	0.082
3	15.595	2788	379	0.054
4	16.040	45268	4786	0.876
5	17.099	7753	1212	0.150
6	17.920	56415	3968	1.092
7	21.517	4551	476	0.088
8	22.033	46077	5028	0.892
9	22.543	4920055	449357	95.211
10	22.992	54181	3190	1.048
11	23.622	19649	1513	0.380
Total		5167527	471585	100.000