


Mass Spectrum

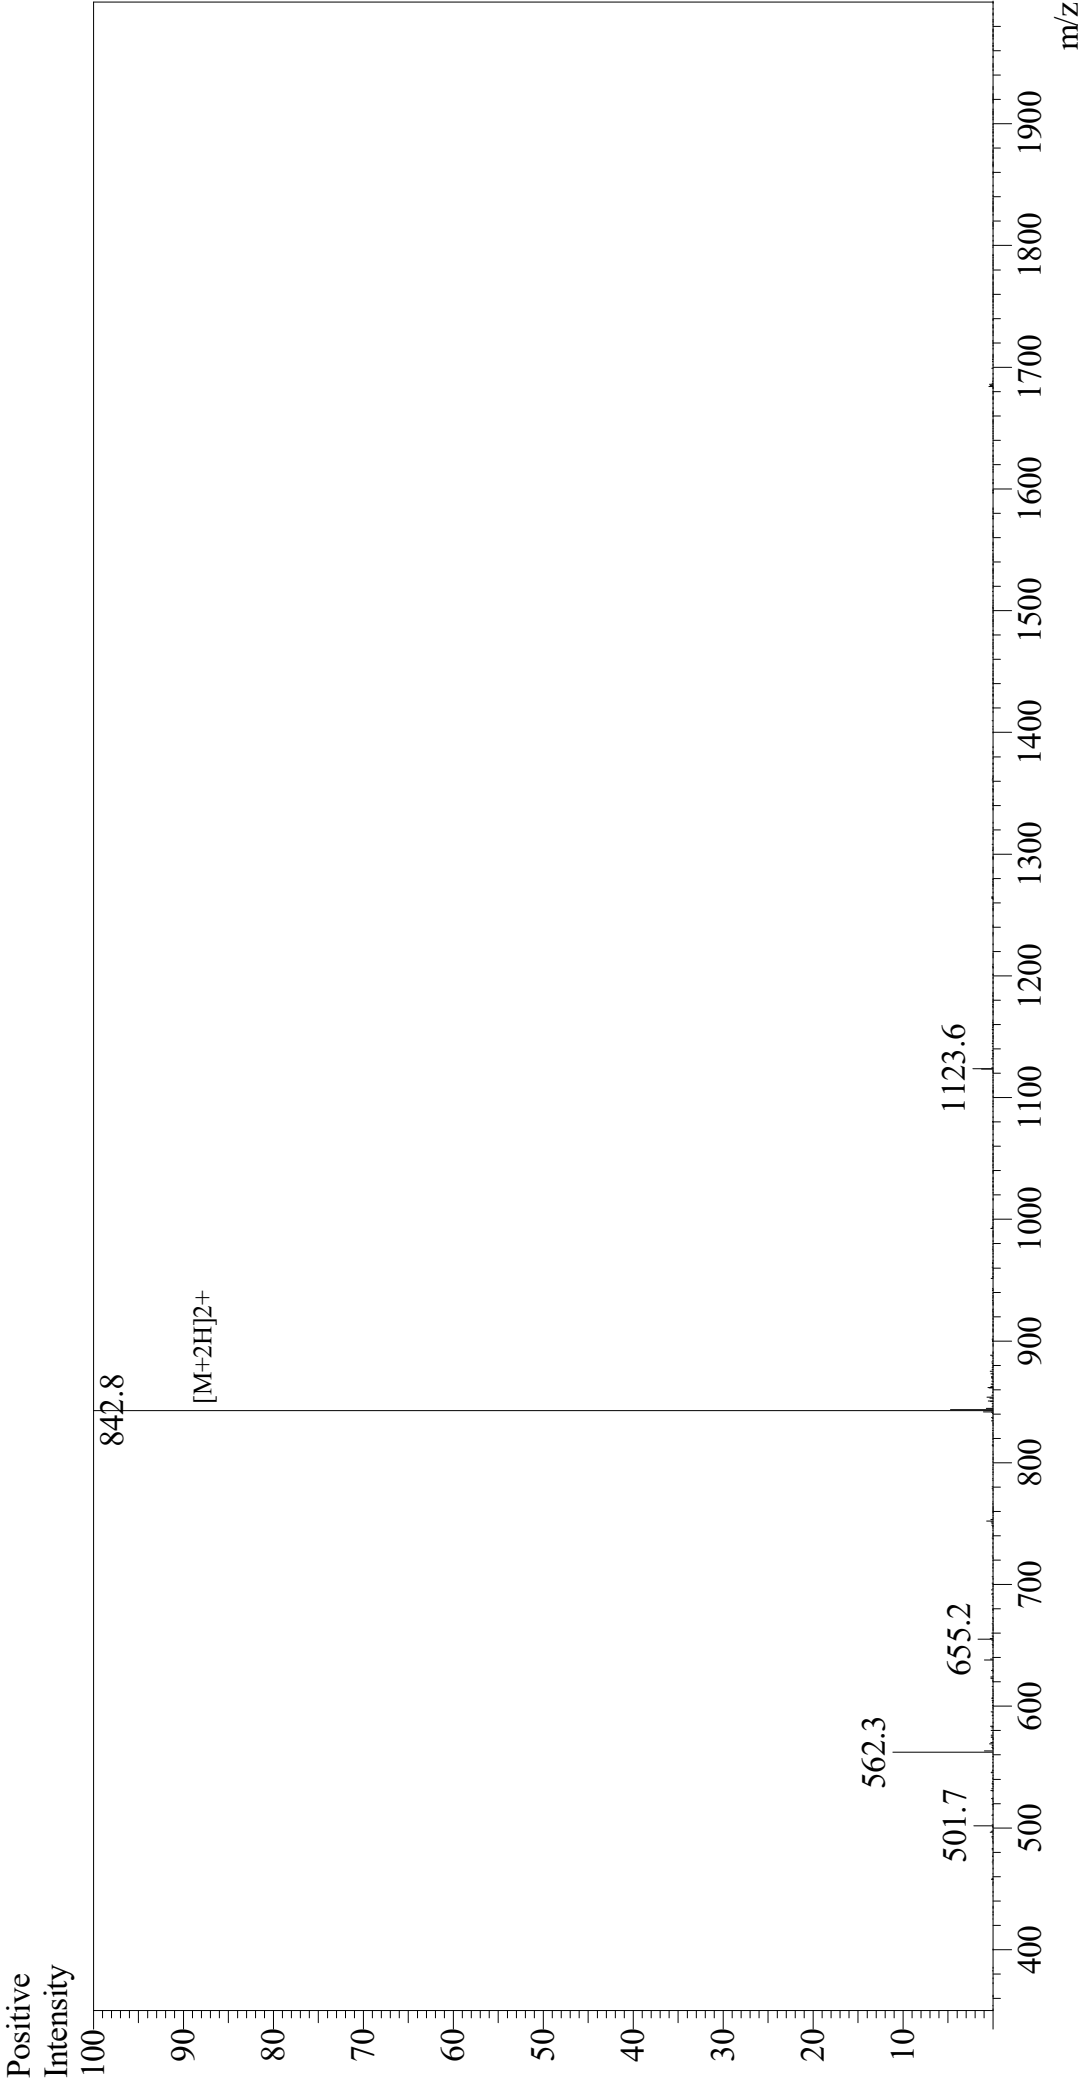

Sample Information
Month-Day Processed : 04/19/21
Time Processed : 7:38:50
Injection Volume : 0.4
Sample Name : α -Factor Mating Pheromone, yeast
Cat No : RP01002
Lot No : E5234321D
Theoretical MW : 1683.98
Observed MW : 1683.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H_2O /50% MeOH