

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat. No. :RP10795
 Lot. No. :E1187019F
 Time Processed : 15:32:06
 Month-Day-Year Processed :06/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
48.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

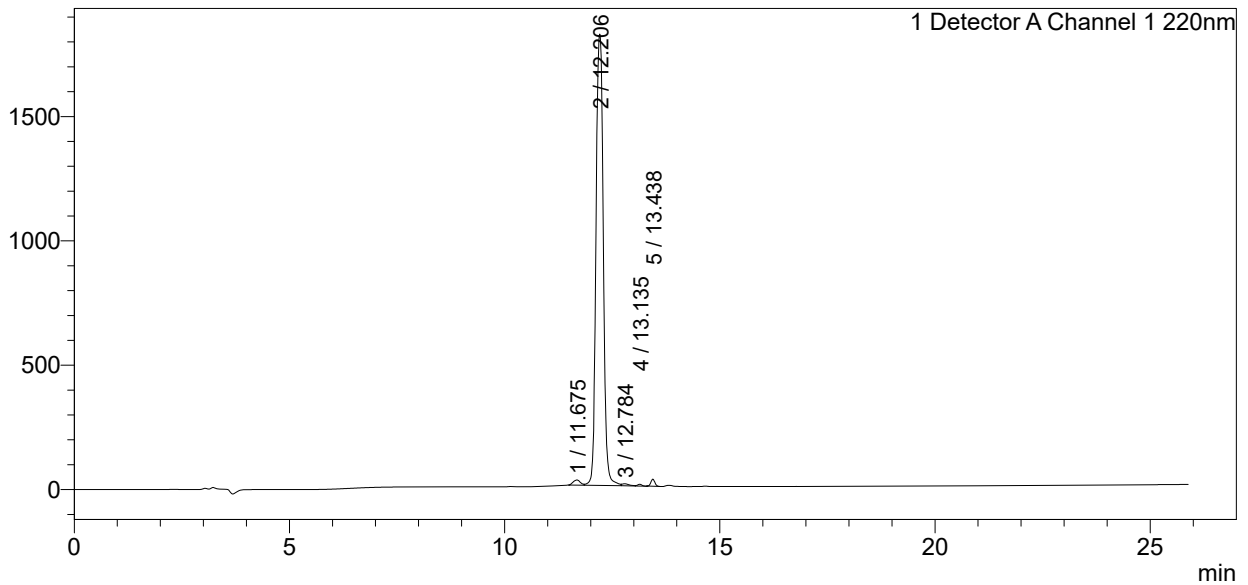

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.675	238440	20699	1.090
2	12.206	21309187	1815062	97.418
3	12.784	95133	8315	0.435
4	13.135	48066	7004	0.220
5	13.438	183047	28586	0.837
Total		21873873	1879666	100.000