

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : E7995620I
 Time Processed : 23:38:41
 Month-Day-Year Processed : 09/25/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

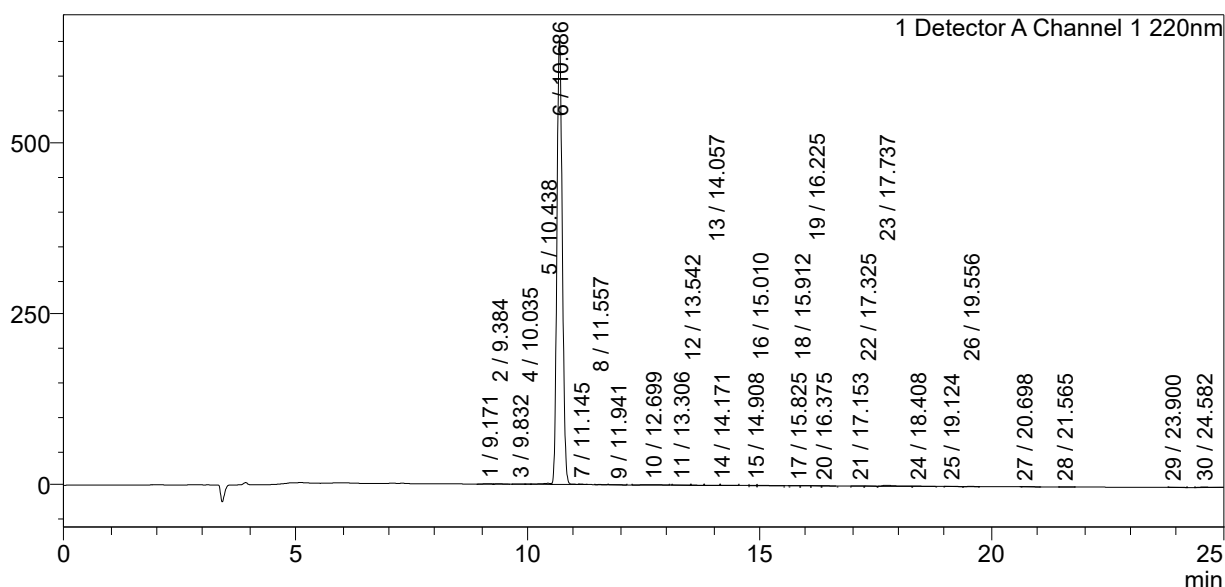

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.171	5426	370	0.101
2	9.384	6005	690	0.111
3	9.832	1994	227	0.037
4	10.035	1780	281	0.033
5	10.438	19750	1475	0.366
6	10.686	5247746	650442	97.350
7	11.145	1854	291	0.034
8	11.557	1557	235	0.029
9	11.941	3125	306	0.058
10	12.699	16284	679	0.302
11	13.306	5163	320	0.096
12	13.542	2163	251	0.040
13	14.057	2777	208	0.052
14	14.171	3561	218	0.066
15	14.908	1829	201	0.034
16	15.010	5806	273	0.108

Peak#	Ret. Time	Area	Height	Area%
17	15.825	1533	146	0.028
18	15.912	1275	169	0.024
19	16.225	2685	310	0.050
20	16.375	2015	220	0.037
21	17.153	3522	306	0.065
22	17.325	2077	212	0.039
23	17.737	24960	1336	0.463
24	18.408	5028	291	0.093
25	19.124	2085	179	0.039
26	19.556	2083	221	0.039
27	20.698	1481	108	0.027
28	21.565	2264	267	0.042
29	23.900	1970	133	0.037
30	24.582	10813	821	0.201
Total		5390609	661186	100.000