

Sample Name: OVA G4 peptide
 Cat. No. : RP20398
 Lot. No. : E2027021C
 Time Processed: 8:03:54
 Month-Day-Year Processed :04/03/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:ZJ19010014

<Chromatogram>

mV

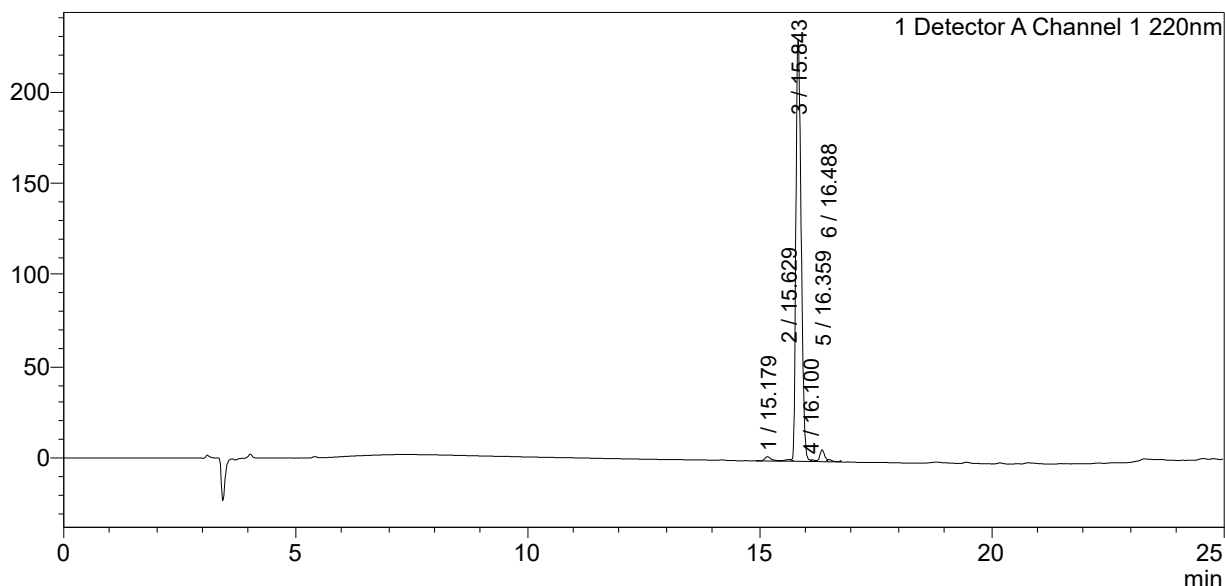

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.179	24677	2444	1.286
2	15.629	9009	915	0.470
3	15.843	1824240	230689	95.082
4	16.100	5880	964	0.306
5	16.359	46718	6462	2.435
6	16.488	8067	1232	0.420
Total		1918593	242706	100.000