

Sample Name :PAR-4 Agonist Peptide, amide
 Cat No :RP11529
 Lot No :E8658320L
 Time Processed :8:25:09 AM
 Month-Day-Year Processed :12/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

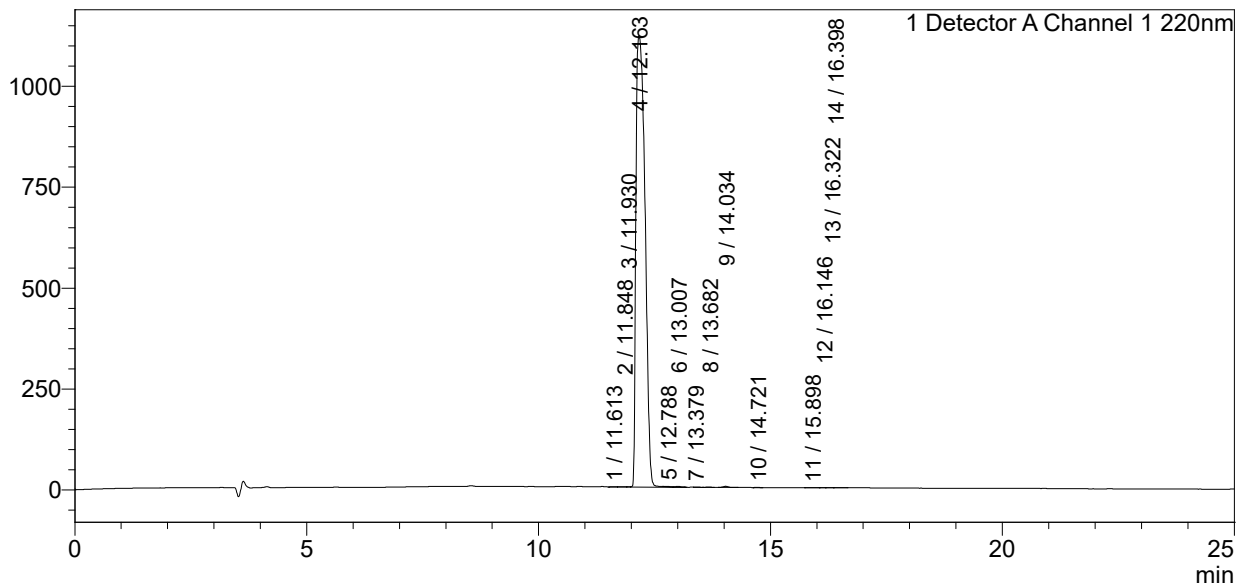

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.613	3608	474	0.024
2	11.848	6579	682	0.043
3	11.930	2844	578	0.019
4	12.163	15186498	1119159	99.554
5	12.788	4134	627	0.027
6	13.007	11282	1898	0.074
7	13.379	1436	156	0.009
8	13.682	2973	493	0.019
9	14.034	21256	2859	0.139
10	14.721	2200	384	0.014
11	15.898	4945	444	0.032
12	16.146	1582	229	0.010
13	16.322	2151	236	0.014
14	16.398	3022	245	0.020
Total		15254509	1128464	100.000