

Sample Name :hgp100(25-33)
 Cat No. :RP20344
 Lot No. :E4921420L
 Time Processed :3:14:50
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

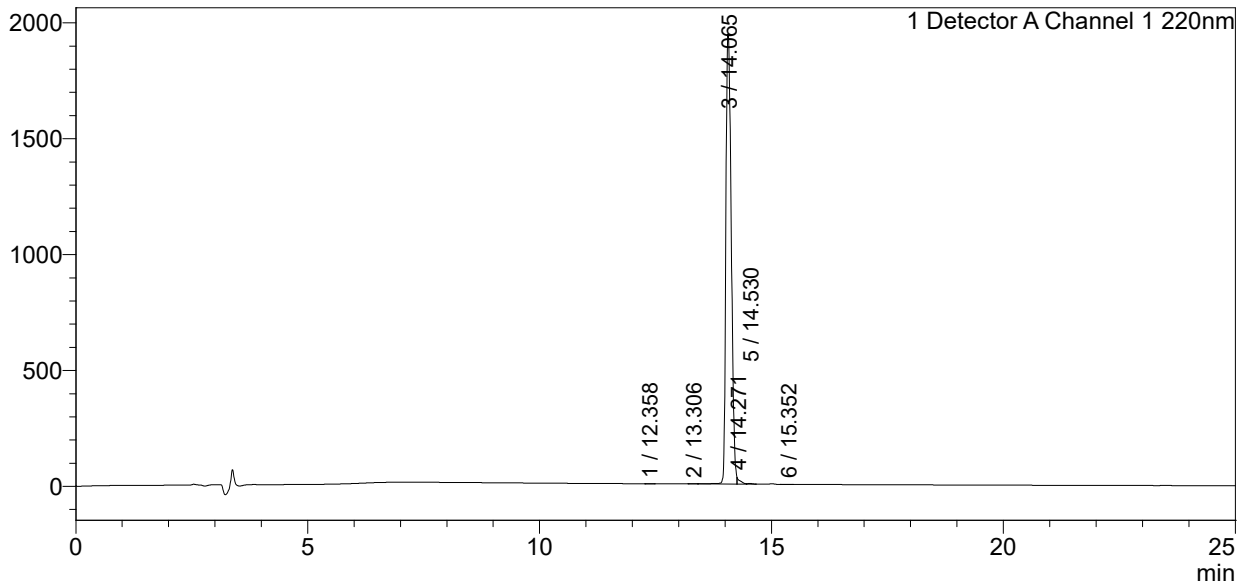

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.358	1571	267	0.010
2	13.306	3714	414	0.024
3	14.065	15600302	1943657	99.114
4	14.271	116283	23887	0.739
5	14.530	16086	2751	0.102
6	15.352	1804	363	0.011
Total		15739761	1971339	100.000