

Sample Name :DYKDDDDK Peptide
 Cat No.: RP10586
 Lot No.: E9272120G
 Time Processed :15:54:43
 Month-Day-Year Processed :07/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
33.00	Pumps	Solvent B Conc.	0
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

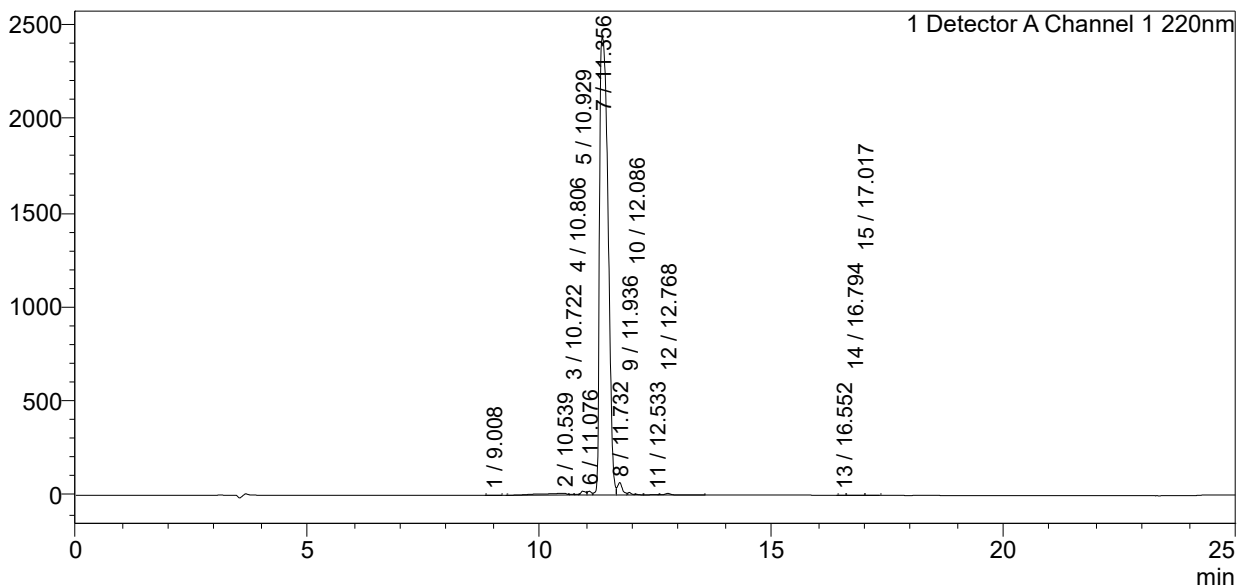

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.008	1990	104	0.006
2	10.539	397403	9742	1.227
3	10.722	29309	4266	0.090
4	10.806	20835	4347	0.064
5	10.929	159533	20795	0.493
6	11.076	120066	20689	0.371
7	11.356	30927633	2433830	95.492
8	11.732	498876	66414	1.540
9	11.936	82065	13418	0.253
10	12.086	28845	4024	0.089
11	12.533	25409	1701	0.078
12	12.768	83366	8735	0.257
13	16.552	1568	178	0.005
14	16.794	7481	417	0.023

Peak#	Ret. Time	Area	Height	Area%
15	17.017	3405	336	0.011
Total		32387784	2588994	100.000