

Sample Name :Hexa-His  
 Cat No. :RP11737  
 Lot No. :E2270521G  
 Time Processed : 17:11:25  
 Month-Day-Year Processed : 07/25/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010017

mV

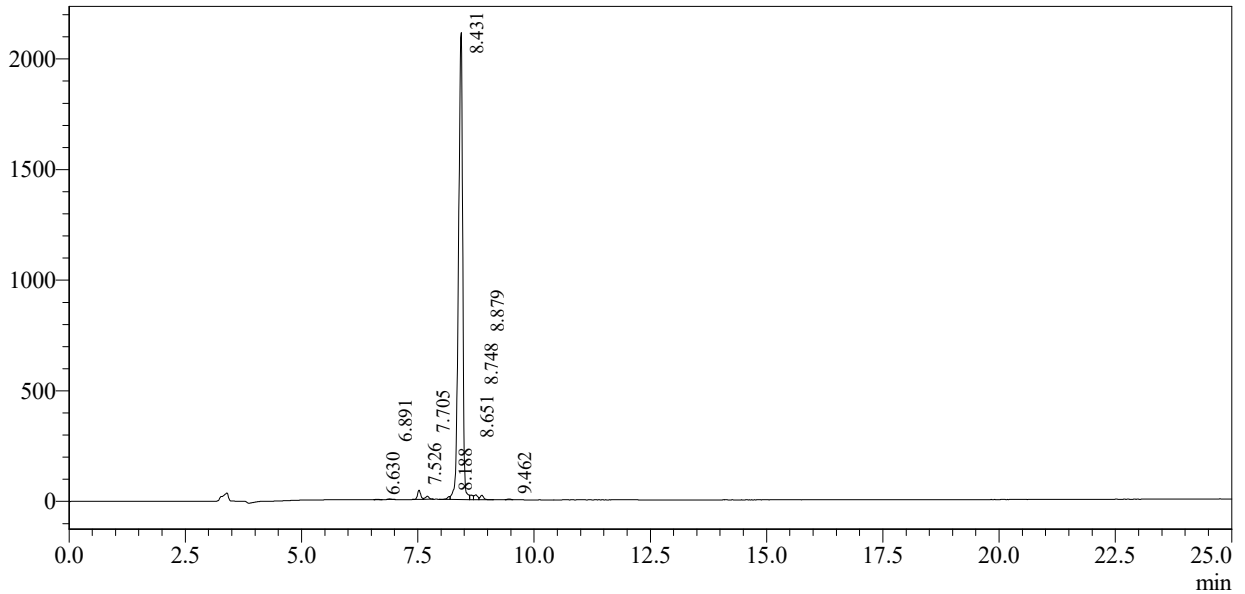

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.630	7670	1755	0.055
2	6.891	12302	2653	0.089
3	7.526	195762	42624	1.411
4	7.705	78763	13655	0.568
5	8.188	57202	13691	0.412
6	8.431	13199587	2110293	95.122
7	8.651	95147	20626	0.686
8	8.748	114800	21502	0.827
9	8.879	102797	20276	0.741
10	9.462	12448	3095	0.090
Total		13876478	2250171	100.000