

Sample Name : CEF20
 Cat. No. : RP11781
 Lot. No. : E4877219I
 Time Processed :14:33:12
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	0	
40.00	Pumps	Pump B Conc.	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

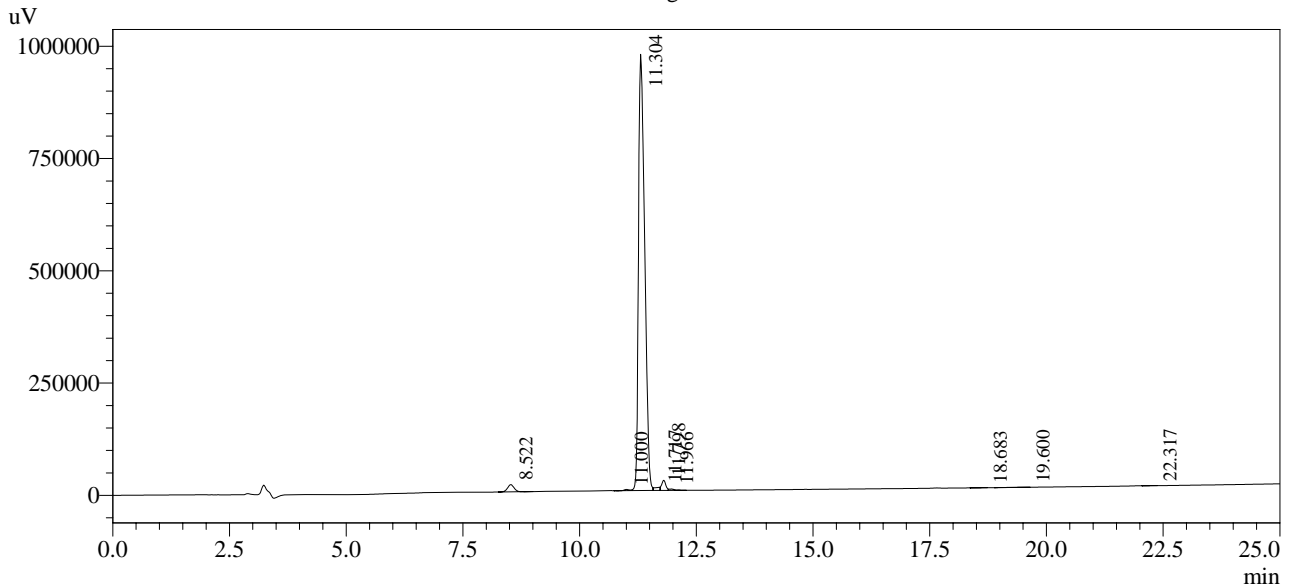

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.522	157027	16156	1.672
2	11.000	19612	2650	0.209
3	11.304	8987286	971554	95.692
4	11.717	57625	7132	0.614
5	11.798	137632	22517	1.465
6	11.966	24947	2926	0.266
7	18.683	746	47	0.008
8	19.600	5910	84	0.063
9	22.317	1061	61	0.011
Total		9391846	1023128	100.000