

Sample Name : MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E5697819F
 Time Processed : 14:10:26
 Month-Day-Year Processed : 07/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

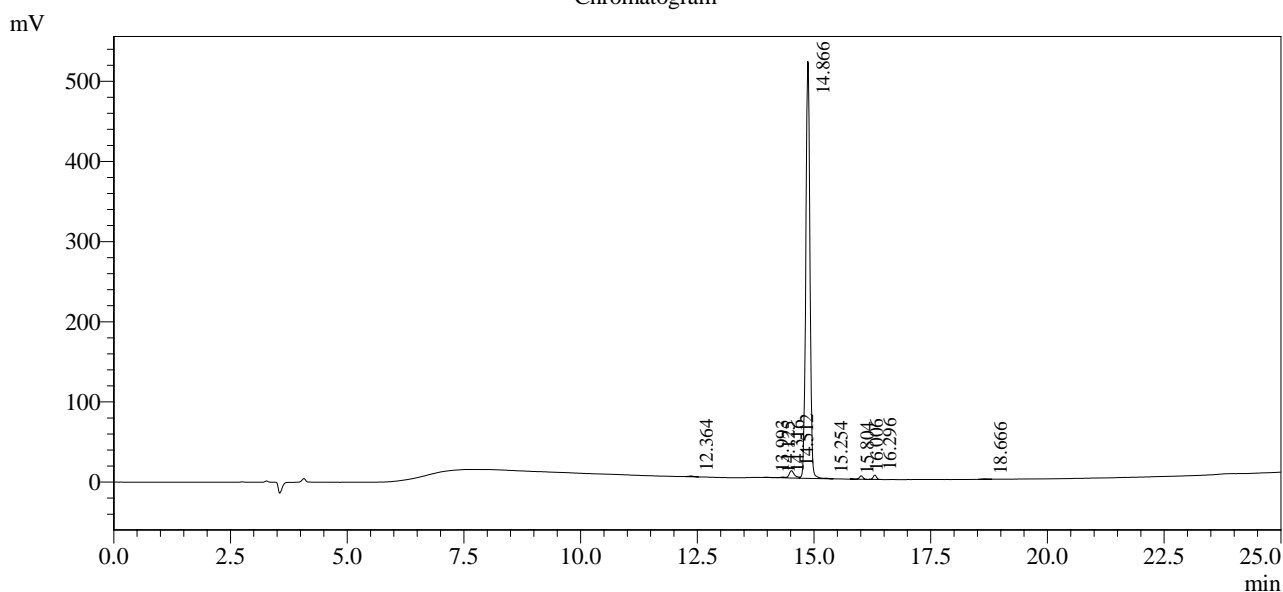

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.364	6521	960	0.195
2	13.993	1164	232	0.035
3	14.125	190	58	0.006
4	14.316	6243	892	0.187
5	14.512	70819	9080	2.119
6	14.866	3201998	520286	95.800
7	15.254	3746	609	0.112
8	15.804	581	207	0.017
9	16.006	21777	4309	0.652
10	16.296	26584	5241	0.795
11	18.666	2757	298	0.082
Total		3342380	542172	100.000