

Sample Name :OVA Peptide (257-264)
 Cat. No. : RP10611
 Lot. No. :E4182319F
 Time Processed :8:26:45
 Month-Day-Year Processed :06/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

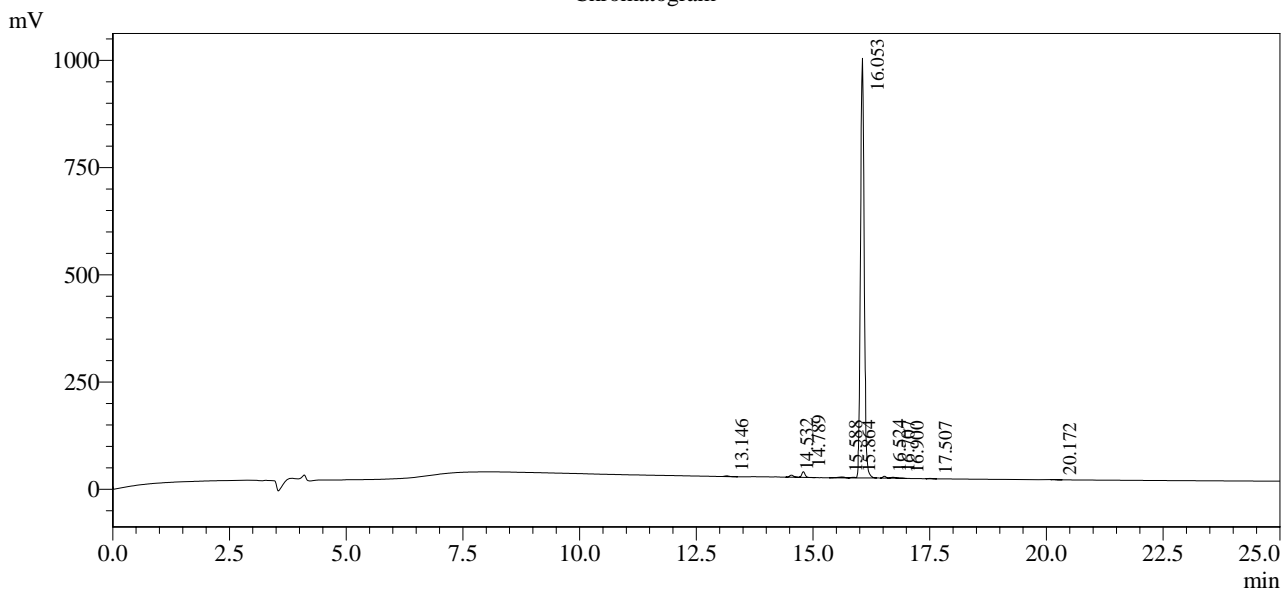

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.146	10920	1621	0.194
2	14.532	30215	4840	0.537
3	14.789	64004	13177	1.138
4	15.588	21229	2070	0.377
5	15.864	8676	1638	0.154
6	16.053	5442796	978415	96.779
7	16.524	20122	4214	0.358
8	16.707	16769	2217	0.298
9	16.900	2492	635	0.044
10	17.507	4507	886	0.080
11	20.172	2201	448	0.039
Total		5623932	1010160	100.000