

Sample Name : PAR-4 Agonist Peptide, amide
 Cat No.: RP11529
 Lot No.: E7021119J
 Time Processed : 7:03:32
 Month-Day-Year Processed : 10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|-----------------|-------|
| 0.01 | Pumps | Solvent B Conc. | 5 |
| 25.00 | Pumps | Solvent B Conc. | 65 |
| 25.01 | Pumps | Solvent B Conc. | 95 |
| 27.00 | Pumps | Solvent B Conc. | 95 |
| 27.01 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Pumps | Solvent B Conc. | 5 |
| 33.00 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

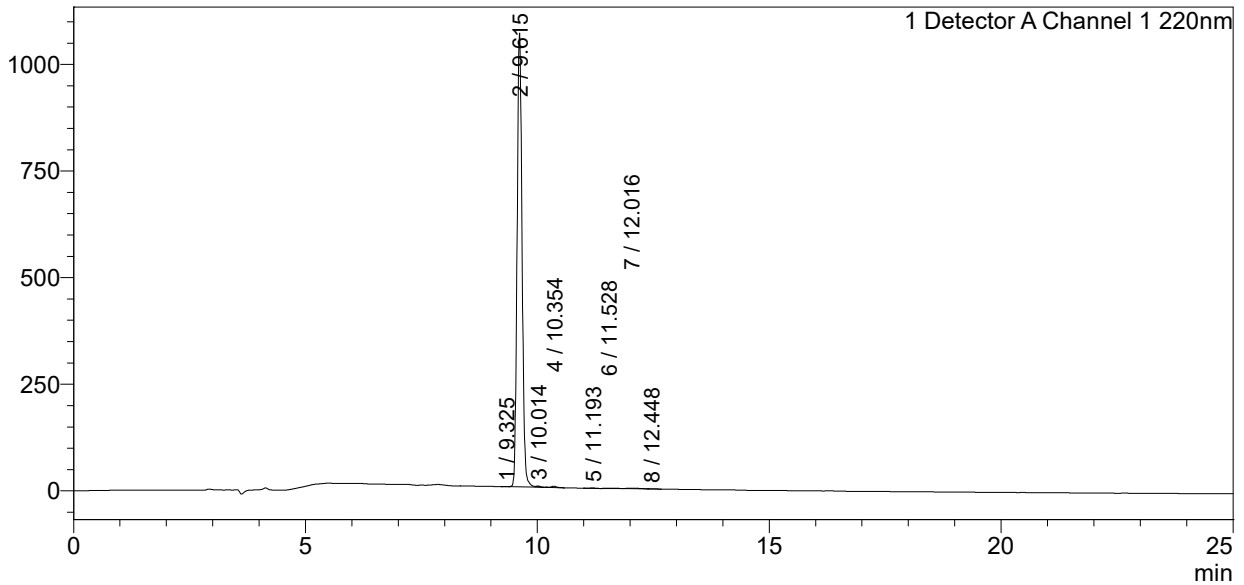

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|---------|---------|
| 1 | 9.325 | 3259 | 461 | 0.041 |
| 2 | 9.615 | 7929263 | 1064844 | 99.172 |
| 3 | 10.014 | 8581 | 1889 | 0.107 |
| 4 | 10.354 | 24206 | 3141 | 0.303 |
| 5 | 11.193 | 9140 | 914 | 0.114 |
| 6 | 11.528 | 5005 | 328 | 0.063 |
| 7 | 12.016 | 14062 | 590 | 0.176 |
| 8 | 12.448 | 1918 | 164 | 0.024 |
| Total | | 7995435 | 1072332 | 100.000 |