

Sample Name :DYKDDDDK Peptide
 Cat No. :RP10586
 Lot No. :E9207220I
 Time Processed :15:02:34
 Month-Day-Year Processed :10/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

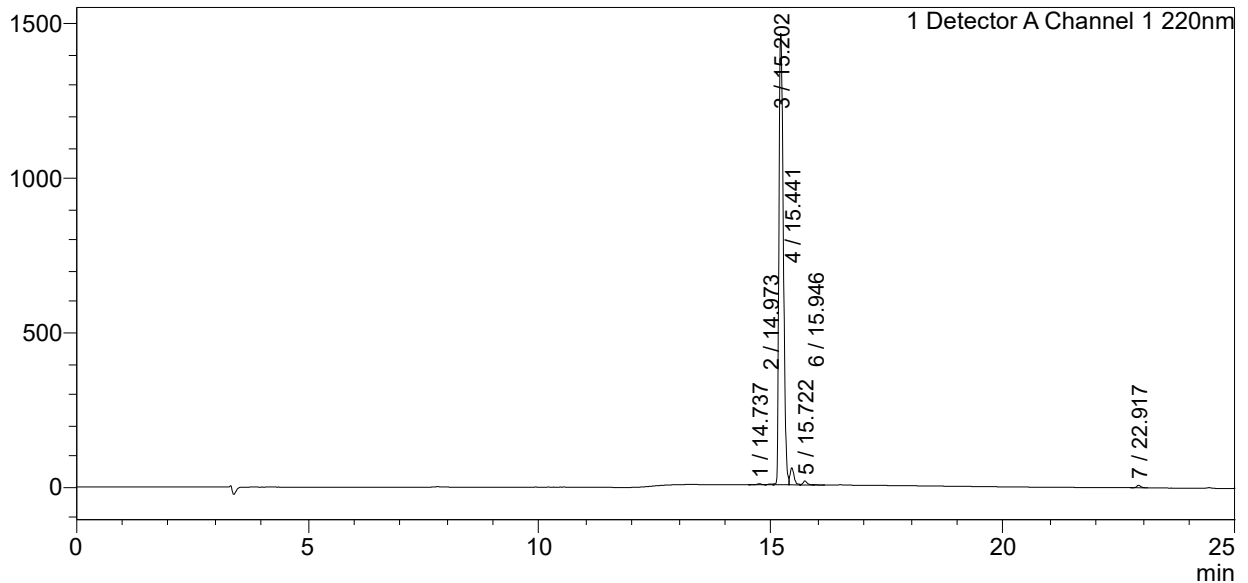

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.737	20867	3550	0.207
2	14.973	15582	2815	0.154
3	15.202	9591543	1463527	95.015
4	15.441	336091	55191	3.329
5	15.722	77142	12839	0.764
6	15.946	5661	1038	0.056
7	22.917	47885	8047	0.474
Total		10094771	1547008	100.000