

Sample Name: OVA Peptide (257-264)  
 Cat No. : RP10611  
 Lot No. : E3716320E  
 Time Processed : 8:25:18  
 Month-Day-Year Processed : 05/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

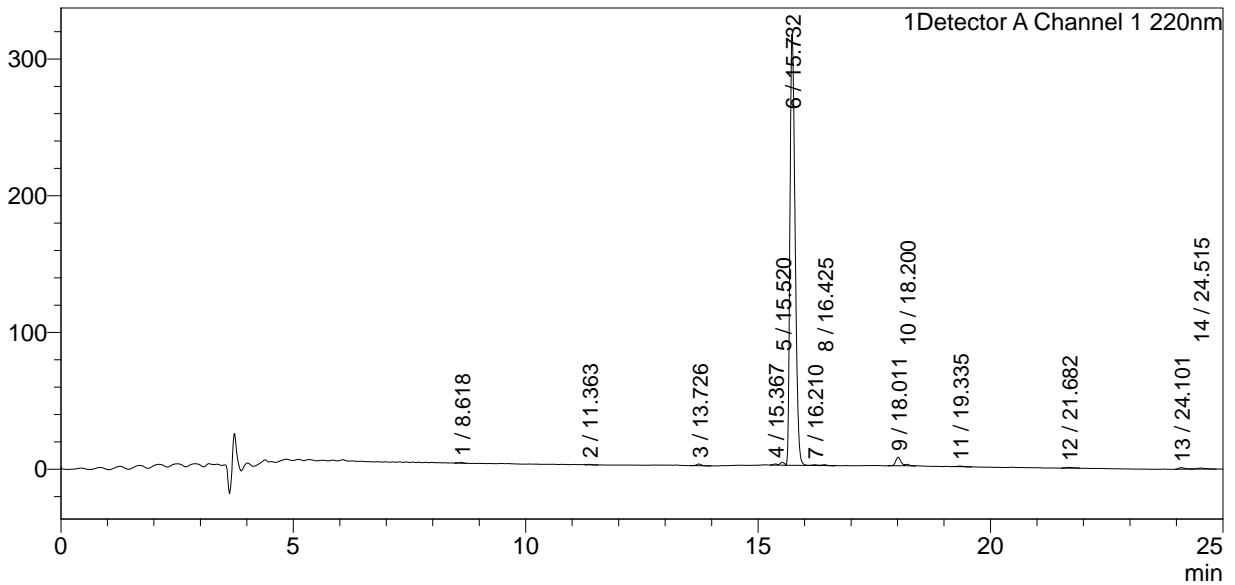

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.618	3423	590	0.134
2	11.363	1662	310	0.065
3	13.726	9230	1306	0.361
4	15.367	5214	821	0.204
5	15.520	13282	2035	0.520
6	15.732	2428521	315144	95.029
7	16.210	4714	534	0.184
8	16.425	4396	649	0.172
9	18.011	46505	6223	1.820
10	18.200	6960	1142	0.272
11	19.335	3539	474	0.138
12	21.682	5470	557	0.214
13	24.101	11876	1101	0.465
14	24.515	10763	753	0.421
Total		2555556	331637	100.000