

Sample Name :Melittin,honey bee
 Cat No. :RP20415
 Lot No. :PE2911901
 Time Processed :16:43:43
 Month-Day-Year Processed :01/31/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

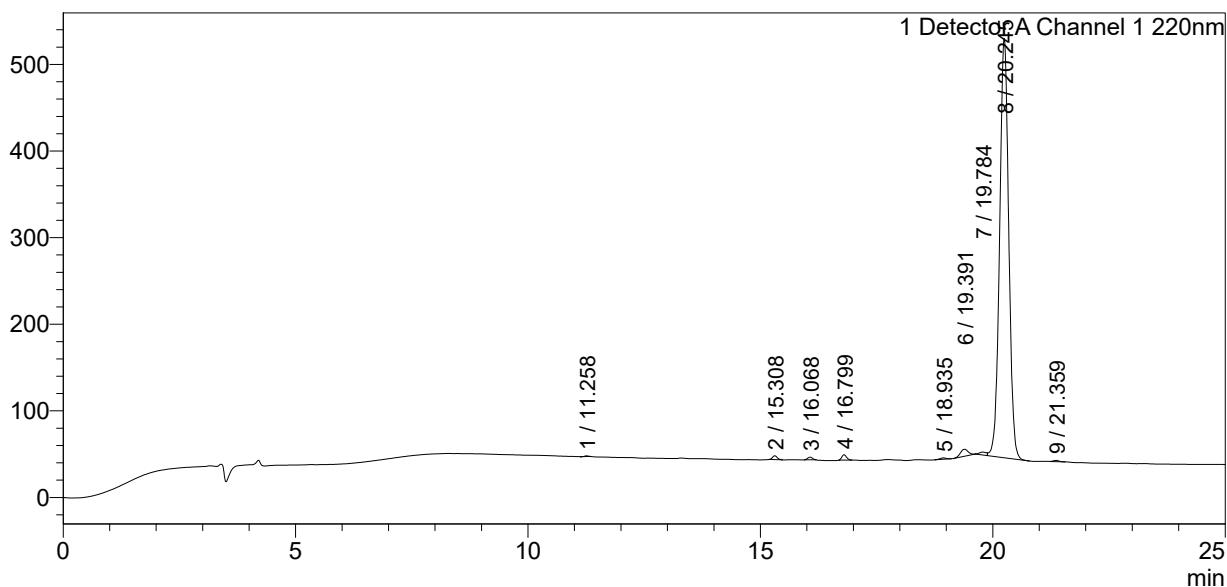

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.258	4074	825	0.060
2	15.308	30651	4401	0.448
3	16.068	21546	3015	0.315
4	16.799	42247	6117	0.618
5	18.935	13588	1508	0.199
6	19.391	97165	8212	1.421
7	19.784	35756	3384	0.523
8	20.245	6583160	484054	96.252
9	21.359	11295	1443	0.165
Total		6839483	512959	100.000