

Sample Name :OVA Peptide (257-264)
 Cat No. :RP10611
 Lot No. :E3599321E
 Time Processed :7:18:46
 Month-Day-Year Processed :05/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

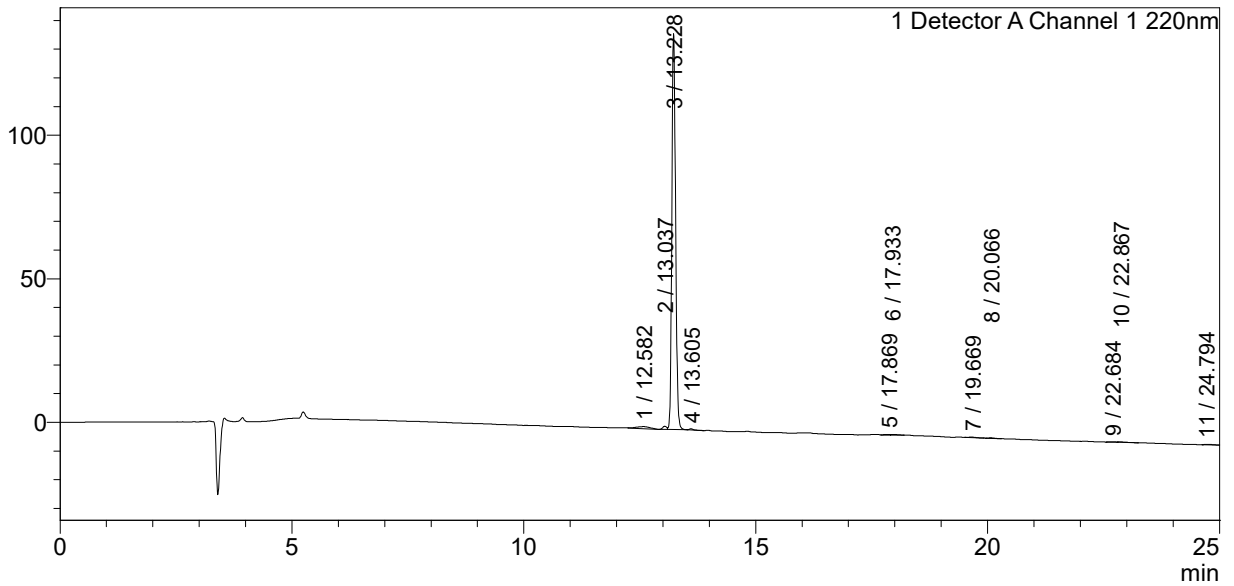

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.582	15911	756	1.946
2	13.037	6538	1120	0.799
3	13.228	778898	137992	95.245
4	13.605	2491	424	0.305
5	17.869	2508	235	0.307
6	17.933	2628	234	0.321
7	19.669	2158	214	0.264
8	20.066	1655	207	0.202
9	22.684	1527	171	0.187
10	22.867	1980	155	0.242
11	24.794	1490	147	0.182
Total		817783	141655	100.000