


Sample Name :RGD
 Cat No.: RP20297
 Lot No.: E6796219J
 Time Processed :17:20:57
 Month-Day-Year Processed :10/25/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>
 Time Module Command Value
 <<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

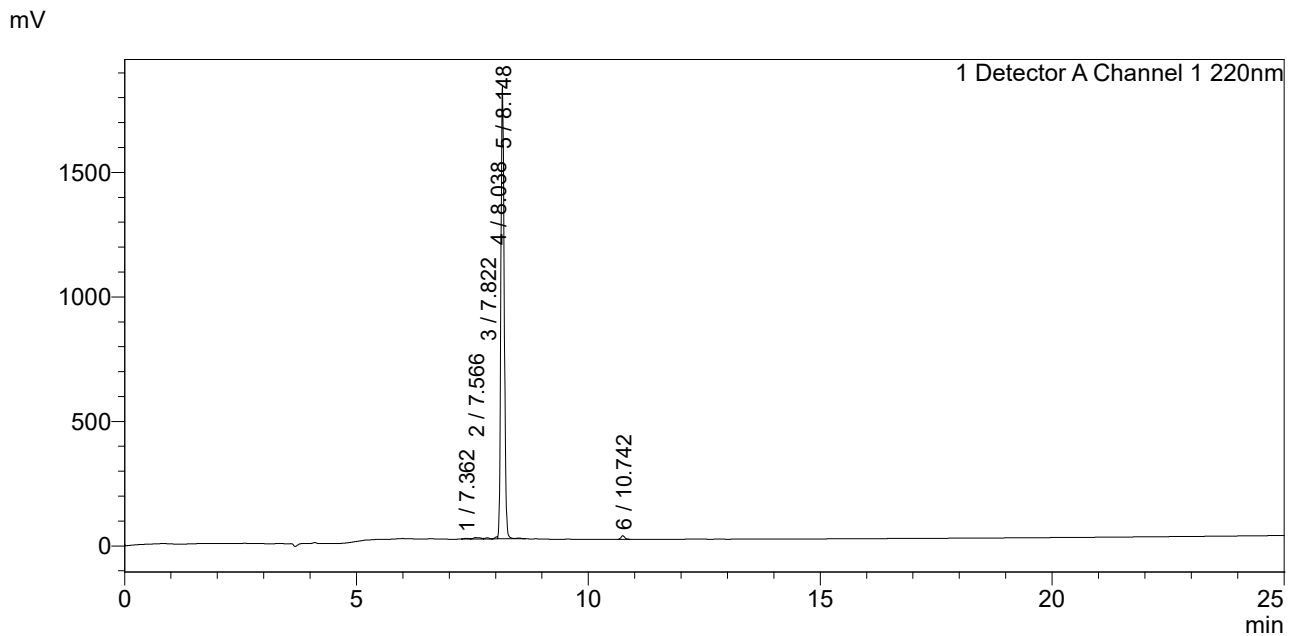

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.362	19838	2843	0.212
2	7.566	57610	5569	0.617
3	7.822	25912	4289	0.277
4	8.038	33731	8450	0.361
5	8.148	912506	1821625	97.696
6	10.742	78163	14546	0.837
Total		9340759	1857322	100.000