


Mass Spectrum

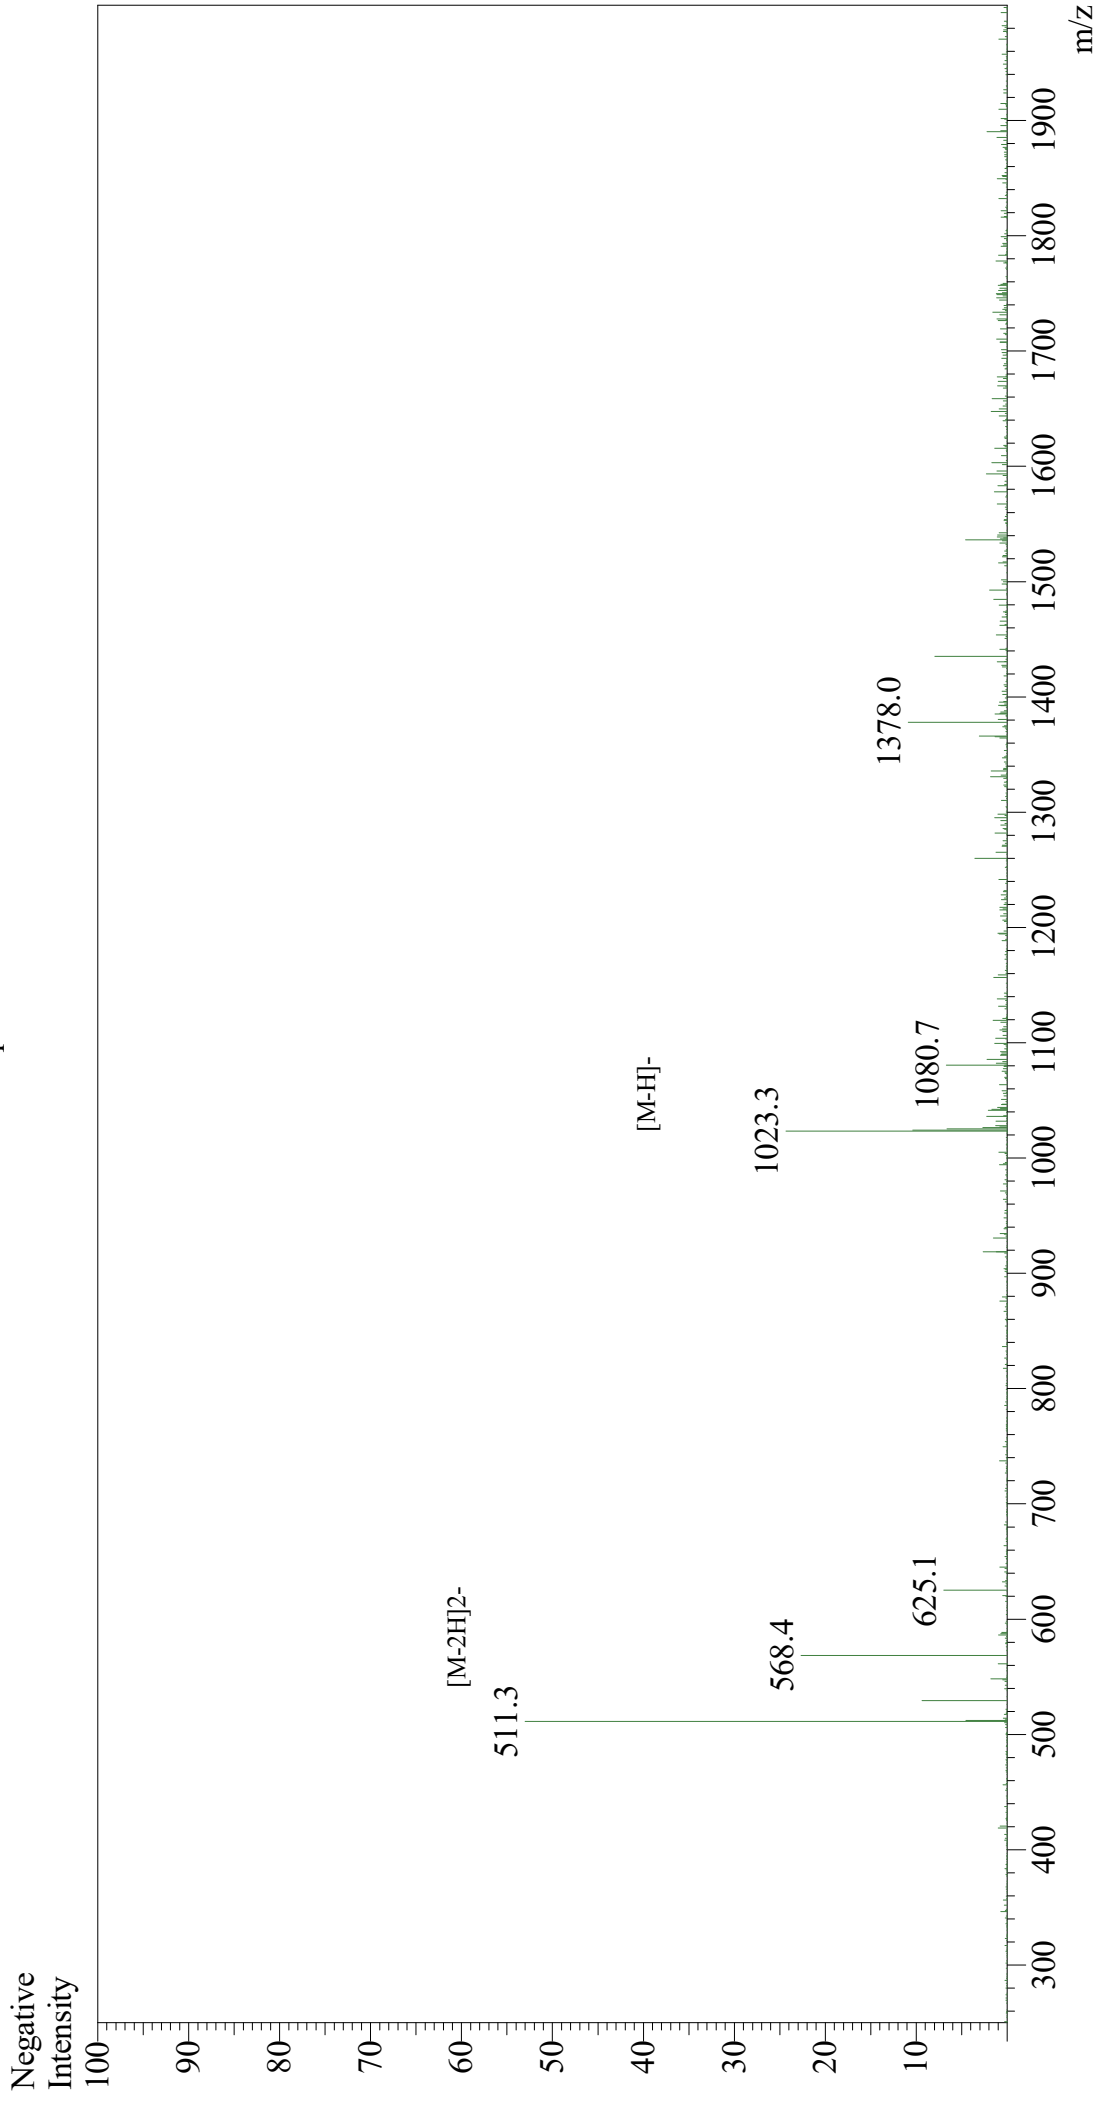

Sample Information

User : Gary
Month-Day Processed : 10/24/19
Time Processed : 09:05:54 AM
Injection Volume : 0.3
Sample Name : RGD
Cat No. : RP20297
Lot No. : E6796219J
Theoretical MW : 1025.06
Observed MW : 1024.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : -3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH