


Mass Spectrum

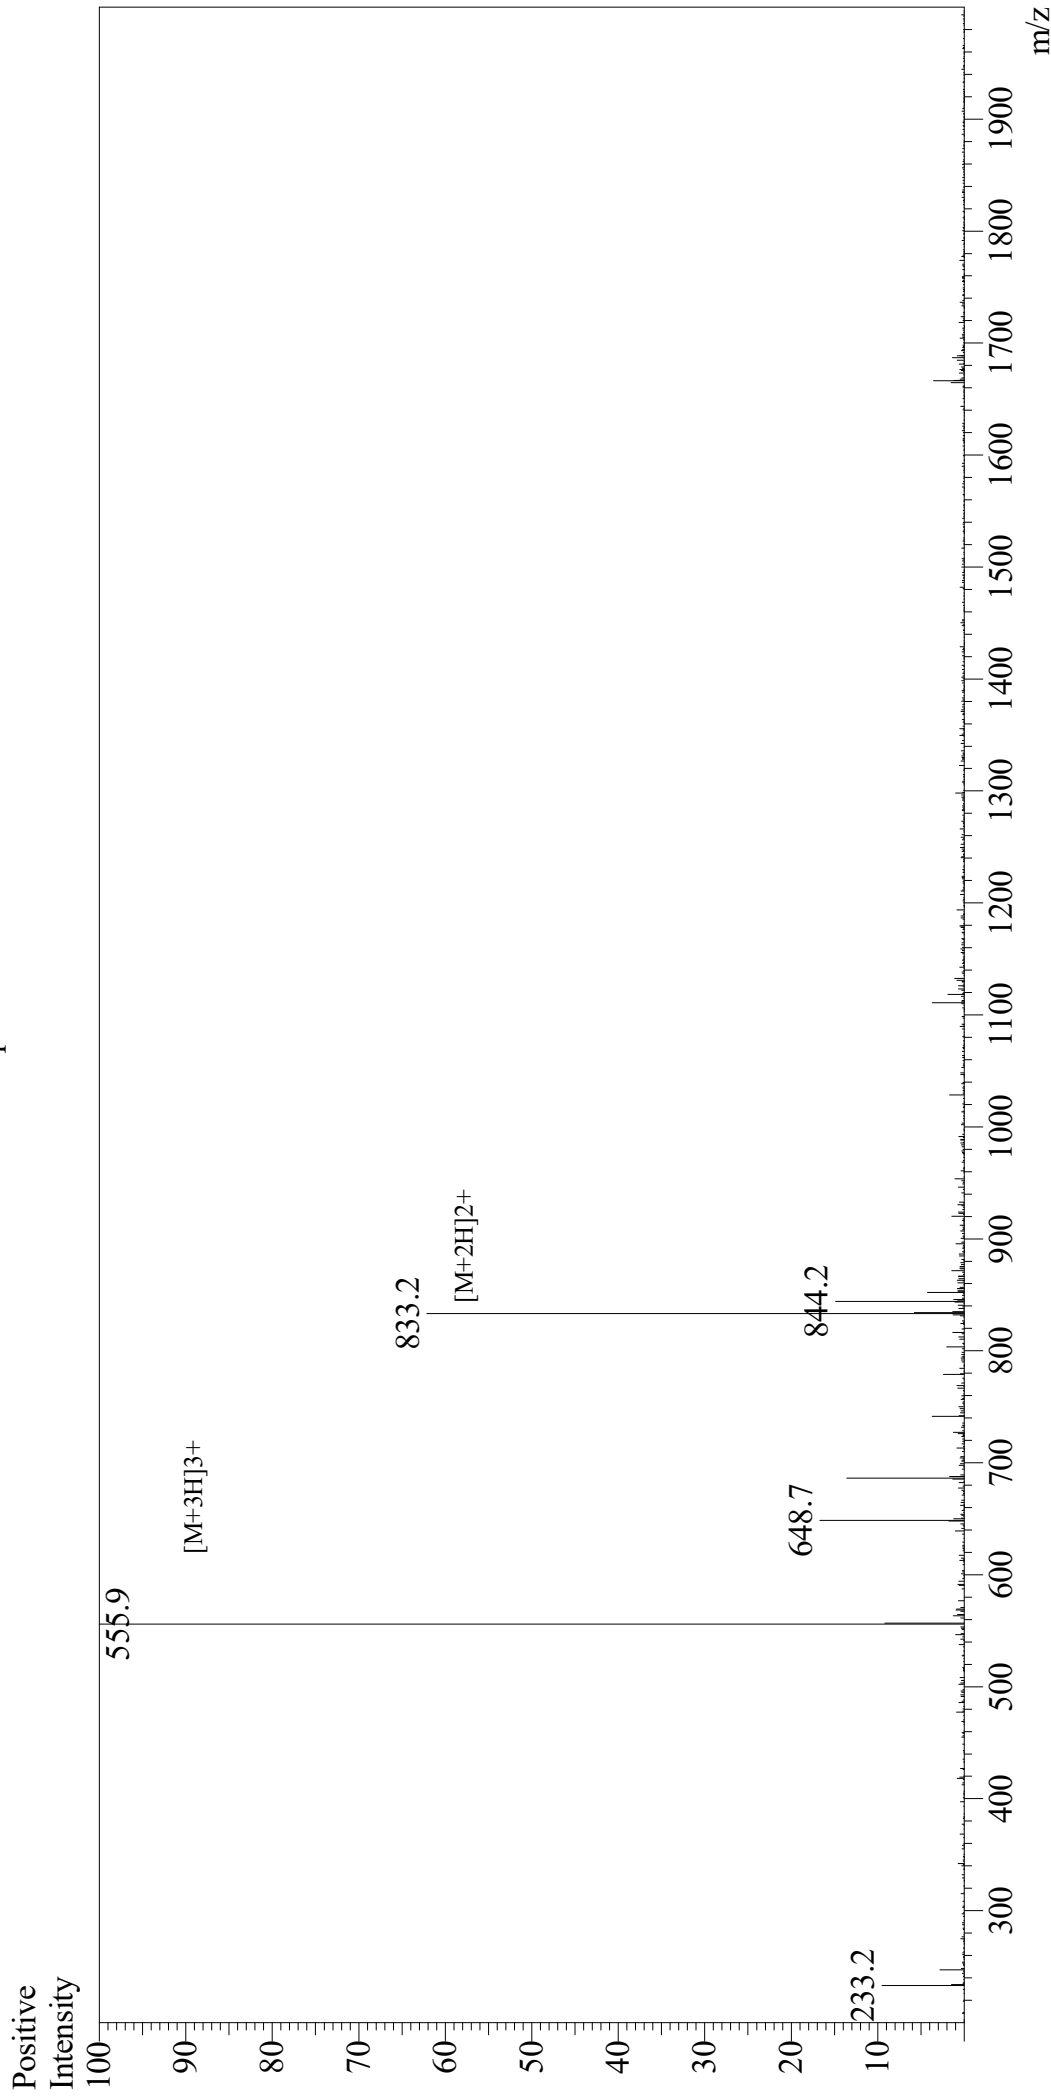

Sample Information

User : Gary
 Month-Day Processed : 10/29/19
 Time Processed : 07:32:18 PM
 Injection Volume : 0.3
 Sample Name : α -Melanocyte-Stimulating Hormone (MSH), amide
 Cat No. : RP10644
 Lot No. : E1709219J
 Theoretical MW : 1664.90
 Observed MW : 1664.7

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : GK11010007
 Interface Bias : +4.5kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2ml/min
 B.conc : 50%H2O/50%MeOH